

FINAL DRAFT
RECOMMENDATION

Draft 1

49th CIML Meeting

Auckland 2014

**SUBMITTED
FOR CIML
APPROVAL**

Revision of R 117-2 (Marked)

Dynamic measuring systems for liquids other than water.

Part 2: Metrological controls and performance tests



ORGANISATION INTERNATIONALE
DE MÉTROLOGIE LÉGALE

INTERNATIONAL ORGANIZATION
OF LEGAL METROLOGY

Co-Secretariats:

Germany

United States

☐ vote (P-members
only) and comments
by:

~~TITLE OF THE 3CD (English):~~

~~R 117-2~~

~~Dynamic mMeasuring Systems for Liquids other than Water~~

~~Part 2: Metrological controls and performance tests~~

~~EXPLANATORY NOTE~~

~~Work originally started on the effort to produce an R117R 117 “test methods” document in the period of 1997—2004. This work was led by Germany and the Netherlands. In 2004, it was decided to delay work on the test methods document until after approval and publication of R117R 117-1 “General Requirements.”~~

~~After publication of R117R 117-1 in 2008, an international working group (IWG) was formed to create R117R 117-2. The United States serves as the chair of the IWG—with significant on-going participation from several other member states. The IWG met several times, and distributed the first committee draft of R117R 117-2 in 2011. In 2012, the IWG was “re-established” as an OIML Project Group (PG) according to the new OIML directives for the technical work and many new project group P-members were added. In addition to the “in-person” meetings, the IWG/PG has also held over 40 web-based meetings to continue to accelerate the work effort.~~

~~The Project Group chair would like to take this opportunity to thank the PG participants for all of their hard work on this document and to thank the nations that have graciously hosted the PG meetings.~~

FEDOR

Some special notes concerning the 2CD, 3CD and the Preliminary Ballot of R117R 117-2:

Because of its size and complexity, this document (R117R 117-2) currently only covers metrological controls and performance tests for type evaluation.

~~There will be an interim period where the testing requirements in R117R 117-1, Annex A (based on OIML D-11:2004) are still allowed, but it is strongly advised to apply the testing requirements of R117R 117-2, Chapter 4 (which are based on D-11:2013). In the immediate revision (of all three parts of R117R 117), these Chapter 4 tests will be the only testing requirements allowed and test level definitions will be moved from R117R 117-2 to R117R 117-1. R117R 117-1 Annex A and R117R 117-2 Chapter 4 will be fully harmonized in the immediate revision of all three parts of R117R 117.~~

~~After receiving international comments on the 1CD (in 2011), the following new items are included with the package that accompanies the 2CD of R117R 117-2:~~

- ~~Responses to international comments on the 1CD;~~
- ~~Annex E – Measuring Systems for Beer + Milk + other foaming potable liquids;~~
- ~~Annex F – Pipelines + Ship Loading Systems; and~~
- ~~Annex G – Aircraft Fueling Systems~~

~~Some newly developed items in this document (R117R 117-2), whenif approved, will necessitate a change to an **amendment** of some of the corresponding “requirements” sections of R117R 117-1. An attempt has been made to clearly mark these items in R117R 117-2. The most significant of these changes will include a replacement the removal of Annex A from R117R 117-1 (to delete test descriptions which are now part of Section 4 of R117R 117-2) and a change that makes endurance testing only relevant for meters with moving parts (Section 5.4).~~

~~Plan to move R117R 117-2 Sections 4.2, 4.8.1, 4.8.2, 4.8.3, 4.8.4, and 4.9.1.1 into R117R 117-1 as part of the immediate revision of all three parts. The concept is to fully harmonize R117R 117-1 and R117R 117-2 in the immediate revision.~~

Foreword

The International Organization of Legal Metrology (OIML) is a worldwide, intergovernmental organization whose primary aim is to harmonize the regulations and metrological controls applied by the national metrological services, or related organizations, of its Member States. The main categories of OIML publications are:

- **International Recommendations (OIML R)**, which are model regulations that establish the metrological characteristics required of certain measuring instruments and which specify methods and equipment for checking their conformity. OIML Member States shall implement these Recommendations to the greatest possible extent;
- **International Documents (OIML D)**, which are informative in nature and which are intended to harmonize and improve work in the field of legal metrology;
- **International Guides (OIML G)**, which are also informative in nature and which are intended to give guidelines for the application of certain requirements to legal metrology;
- **International Basic Publications (OIML B)**, which define the operating rules of the various OIML structures and systems; and

OIML Draft Recommendations, Documents and Guides are developed by Project Groups linked to Technical Committees or Subcommittees which comprise representatives from OIML Member States. Certain international and regional institutions also participate on a consultation basis. Cooperative agreements have been established between the OIML and certain institutions, such as ISO and the IEC, with the objective of avoiding contradictory requirements. Consequently, manufacturers and users of measuring instruments, test laboratories, etc. may simultaneously apply OIML publications and those of other institutions.

International Recommendations, Documents, Guides and Basic Publications are published in English (E) and translated into French (F) and are subject to periodic revision.

Additionally, the OIML publishes or participates in the publication of **Vocabularies (OIML V)** and periodically commissions legal metrology experts to write **Expert Reports (OIML E)**. Expert Reports are intended to provide information and advice, and are written solely from the viewpoint of their author, without the involvement of a Technical Committee or Subcommittee, nor that of the CIML. Thus, they do not necessarily represent the views of the OIML.

This publication, ~~R 117~~OIML R 117-2, edition 201X (E) – was developed by the OIML Technical Subcommittee TC 8/SC 3 *Dynamic measurement of liquids other than water*. It was approved for final publication by the International Committee of Legal Metrology in 201X at its xxth meeting in xxxx, in month/year and will be submitted to the International Conference on Legal Metrology in 2016 for formal sanction.

OIML Publications may be downloaded from the OIML web site in the form of PDF files. Additional information on OIML Publications may be obtained from the Organization's headquarters:

Bureau International de Métrologie Légale
11, rue Turgot - 75009 Paris - France
Telephone: 33 (0)1 48 78 12 82
Fax: 33 (0)1 42 82 17 27
E-mail: biml@oiml.org
Internet: www.oiml.org

FEDOR

Contents

1	Scope	14
2	Metrological control	15
2.1	Type evaluation and approval.....	15
2.2	Initial verification	16
3	Symbols, units and equations	16
4	Type evaluation performance tests	21
4.1	General	21
4.2	Measurement uncertainty	22
4.3	Reference conditions	22
4.4	Test quantities.....	22
4.5	Preventing the liquid temperature from influencing test results.....	23
4.6	Software setting / configuration	24
4.7	Reverse flow (from OIML R 117-1, 2.13.4)	24
4.8	Disturbance and influence factor tests - climatic and mechanical environmental conditions	24
4.9	Disturbance and influence factor tests – electrical tests	32
4.10	Tests for EUTs powered by a road vehicle battery.....	52
5	Testing procedures for meter sensors and measuring devices	56
5.1	General information.....	56
5.2	Test equipment	58
5.3	Accuracy.....	59
5.4	Endurance test	64
5.5	Accuracy on the minimum measured quantity	65
5.6	Additional testing procedures for electronic measuring devices (sensor + transducer)	66
6	Testing procedures for electronic calculators (that may be equipped with a conversion device), indicating devices, and associated devices.....	69
6.1	General information.....	69
6.2	Electronic calculators and indicating devices.....	72
6.3	Conversion device (as part of an electronic calculator).....	73
6.4	Associated measuring devices.....	77
6.5	Temperature conversion: Tests on the response time of the measuring system temperature sensor.....	78
7	Testing procedures for gas elimination devices	79
7.1	General information.....	79
7.2	Testing	80
8	Test procedures for ancillary devices	91
8.1	General information.....	91
8.2	Disturbance and influence factor tests for ancillary devices	92
8.3	Printing devices	93
8.4	Memory device (e.g. data storage device- DSD).....	94
8.5	Conversion devices.....	95
A.1	General information.....	96
A.2	Testing procedures for meters.....	97
A.3	Testing procedures for electronic devices: calculator, correction, indicating and associated devices.....	98
A.4	Testing procedures for gas elimination	99

A.5	Testing procedures for ancillary devices	99
A.6	Additional testing procedures for complete fuel dispensers	99
A.6.1	General requirements.....	99
A.6.2	Testing procedure related to flow interruption – with maximum specified hose length – only when mechanical calculator is used.....	99
A.6.3	Testing procedures related to fuel dispenser hoses.....	100
A.6.4	Other fuel dispenser functionality to be tested	100
A.6.5	Additional testing for blend dispensers – see OIML R 117-1, 5.9	103
A-L.1	General information.....	105
A-L.2	Testing procedures for meters.....	106
A-L.2.1	Accuracy tests.....	106
A-L.2.2	Tests on the MMQ (with maximum specified hose length if applicable)	106
A-L.2.3	Endurance testing - see OIML R 117-2, 5.4.....	107
A-L.2.4	Check of reverse flow prevention.....	107
A-L.3	Testing procedures for electronic devices: calculator, correction, indicating, and associated devices	107
A-L.4	Testing procedures for gas elimination	107
A-L.5	Testing procedures for ancillary devices	107
A-L.6	Additional testing procedures for complete LPG dispensers	107
A-L.6.1	General requirements.....	107
A-L.6.2	Testing procedure related to flow interruption – with maximum specified hose length – only when mechanical calculator is used.....	108
A-L.6.3	Testing procedures related to LPG dispenser hoses	108
A-L.6.4	Other LPG dispenser functionality to be tested.....	109
B.1	General information.....	115
B.2	Metrological controls and performance tests for type evaluation of the constituent elements	116
B.2.1	Testing procedures for meter sensors, measuring devices and meters with mechanical indicating devices	116
B.2.2	Testing procedures for electronic devices: calculator, correction, indicating, and associated devices	116
B.2.3	Testing procedures for gas elimination devices.....	116
B.2.4	Testing procedures for ancillary devices	116
B.3	Metrological controls and performance tests of the complete measuring system	116
B.3.1	Accuracy test of the complete measuring system.....	116
B.3.2	Complete emptying of the compartment of a road tanker (single compartment trucks only) – See also 7.....	116
B.3.3	Connecting of an empty compartment (multiple compartment trucks only).....	117
B.3.4	Variation in the internal volume of the hose (full hose measuring systems only).....	117
E.1	General information.....	120
E.2	Tests for meter sensors, measuring devices and meters with mechanical indicating devices.....	120
E.3	Tests for electronic devices (calculator, correction device, indicating device, associated devices)	121
E.4	Tests for air/gas elimination devices	122
E.4.1	Air elimination devices for MS for milk	122
E.4.2	Gas elimination devices for MS for beer and other foaming potable liquids	122

E.5	Tests for ancillary devices.....	123
E.6	Additional tests on the complete MS.....	123
E.6.1	MS for milk	123
E.6.2	MS for beer and other foaming liquids.....	133
E.7	Hose variation (see OIML R 117-1, 2.15)	139
F.1	General information.....	140
F.1.1	Type approval.....	140
F.2	Metrological controls and performance tests for type evaluation.....	140
F.2.1	Testing procedures for meter sensors, measuring devices and meters with mechanical indicating devices	140
F.2.2	Testing procedures for electronic devices: calculator, correction, indicating, and associated devices	141
F.2.3	Testing procedures for ancillary devices	141
G.1	General information.....	142
G.2	Metrological controls and performance tests for type approval.....	142
G.2.1	Testing procedures for meter sensors, measuring devices and meters with mechanical indicating devices	142
G.2.2	Testing procedures for electronic devices: calculator, correction, indicating, and associated devices	142
G.2.3	Testing procedures for gas elimination devices.....	143
G.2.4	Testing procedures for ancillary devices	143
G.2.5	Additional test procedures for the complete measuring system intended for the fuelling of aircraft	143
X.2	Chapter 2.....	145
X.5	Chapter 5 (Testing procedures for meter sensors and measuring devices).....	149
X.7	Advice Annex for Section 7 “Test procedures for gas elimination devices”.....	155
1	Scope.....	7
2	Metrological control.....	9
2.1	Type evaluation and approval.....	9
2.2	Initial verification	10
3	Symbols, units and equations	10
4	Type evaluation performance tests	15
4.1	General	15
4.2	Measurement uncertainty	16
4.3	Reference conditions	16
4.4	Test quantities.....	16
4.5	Preventing the liquid temperature from influencing test results.....	16
4.6	Software setting / configuration	17
4.7	Reverse flow (from OIML R 117-1, 2.13.4)	17
4.8	Disturbance and influence factor tests — climatic and mechanical environmental conditions....	17
4.9	Disturbance and influence factor tests — electrical tests	25
4.10	Tests for EUTs powered by a road vehicle battery.....	48
5	Testing procedures for meter sensors and measuring devices	53
5.1	General information.....	53
5.2	Test equipment	55
5.3	Accuracy.....	56
5.4	Endurance test	60

5.5	Accuracy on the minimum measured quantity	61
5.6	Additional testing procedures for electronic measuring devices (sensor + transducer)	62
6	Testing procedures for electronic calculators (that may be equipped with a conversion device), indicating devices, and associated devices	64
6.1	General information	64
6.2	Electronic calculators and indicating devices	66
6.3	Conversion device (as part of an electronic calculator)	68
6.4	Associated measuring devices	72
6.5	Temperature conversion: Tests on the response time of the measuring system temperature sensor	73
7	Testing procedures for gas elimination devices	74
7.1	General information	74
7.2	Testing	75
8	Test procedures for ancillary devices	86
8.1	General information	86
8.2	Disturbance and influence factor tests for ancillary devices	87
8.3	Printing devices	88
8.4	Memory device (e.g. data storage device DSD)	89
8.5	Conversion devices	90
A.1	General information	91
A.2	Testing procedures for meters	92
A.3	Testing procedures for electronic devices: calculator, correction, indicating and associated devices	93
A.4	Testing procedures for gas elimination	93
A.5	Testing procedures for ancillary devices	93
A.6	Additional testing procedures for complete fuel dispensers	93
A.6.1	General requirements	93
A.6.2	Testing procedure related to flow interruption — with maximum specified hose length — only when mechanical calculator is used	93
A.6.3	Testing procedures related to fuel dispenser hoses	95
A.6.4	Other fuel dispenser functionality to be tested	95
A.6.5	Additional testing for blend dispensers — see OIML R 117-1, 5.9	98
A-L.1	General information	100
A-L.2	Testing procedures for meters	101
A-L.2.1	Accuracy tests	101
A-L.2.2	Tests on the MMQ (with maximum specified hose length if applicable)	101
A-L.2.3	Endurance testing — see OIML R 117-2, 5.4	102
A-L.2.4	Check of reverse flow prevention	102
A-L.3	Testing procedures for electronic devices: calculator, correction, indicating, and associated devices	102
A-L.4	Testing procedures for gas elimination	102
A-L.5	Testing procedures for ancillary devices	102
A-L.6	Additional testing procedures for complete LPG dispensers	102
A-L.6.1	General requirements	102
A-L.6.2	Testing procedure related to flow interruption — with maximum specified hose length — only when mechanical calculator is used	103

A.L.6.3	Testing procedures related to LPG dispenser hoses	103
A.L.6.4	Other LPG dispenser functionality to be tested	104
B.1	General information	110
B.2	Metrological controls and performance tests for type evaluation of the constituent elements	111
B.2.1	Testing procedures for meter sensors, measuring devices and meters with mechanical indicating devices	111
B.2.2	Testing procedures for electronic devices: calculator, correction, indicating, and associated devices	111
B.2.3	Testing procedures for gas elimination devices	111
B.2.4	Testing procedures for ancillary devices	111
B.3	Metrological controls and performance tests of the complete measuring system	111
B.3.1	Accuracy test of the complete measuring system	111
B.3.2	Complete emptying of the compartment of a road tanker (single compartment trucks only) – See also 7.	111
B.3.3	Connecting of an empty compartment (multiple compartment trucks only)	112
B.3.4	Variation in the internal volume of the hose (full hose measuring systems only)	112
E.1	General information	115
E.2	Tests for meter sensors, measuring devices and meters with mechanical indicating devices	115
E.3	Tests for electronic devices (calculator, correction device, indicating device, associated devices)	116
E.4	Tests for air/gas elimination devices	117
E.4.1	Air elimination devices for MS for milk	117
E.4.2	Gas elimination devices for MS for beer and other foaming potable liquids	117
E.5	Tests for ancillary devices	118
E.6	Additional tests on the complete MS	118
E.6.1	MS for milk	118
E.6.2	MS for beer and other foaming liquids	129
E.7	Hose variation (see OIML R 117-1, 2.15)	134
F.1	General information	135
F.1.1	Type approval	135
F.2	Metrological controls and performance tests for type evaluation	135
F.2.1	Testing procedures for meter sensors, measuring devices and meters with mechanical indicating devices	135
F.2.2	Testing procedures for electronic devices: calculator, correction, indicating, and associated devices	136
F.2.3	Testing procedures for ancillary devices	136
G.1	General information	137
G.2	Metrological controls and performance tests for type approval	137
G.2.1	Testing procedures for meter sensors, measuring devices and meters with mechanical indicating devices	137
G.2.2	Testing procedures for electronic devices: calculator, correction, indicating, and associated devices	137
G.2.3	Testing procedures for gas elimination devices	138
G.2.4	Testing procedures for ancillary devices	138

G.2.5	Additional test procedures for the complete measuring system intended for the fuelling of aircraft	138
X.2	Chapter 2	140
X.5	Chapter 5 (Testing procedures for meter sensors and measuring devices)	145
X.5	Advice on Chapter 5 concerning meter types	147
X.7	Advice Annex for Section 7 “Test procedures for gas elimination devices”	150

DRAFT

R 117 <u>OIML R 117</u> -2 Annex List	Test p <u>P</u> rocedures for C <u>C</u> omplete M <u>M</u> easuring S <u>S</u> ystems
A and A-LPG	Annex A <u>A</u> Fuel dispensers <u>Blend dispensers</u> ----- Annex A- LPG <u>LPG</u> Fuel dispensers for liquefied gases under pressure <u>(LPG dispensers)</u>
B	Measuring systems on road tankers
C*	<i>Measuring systems for the unloading of ships' tanks and for rail and road tankers using an intermediate tank</i>
D*	<i>Measuring systems for liquefied gases under pressure (other than LPG dispensers)</i>
E	Measuring systems for milk, beer, and other foaming potable liquids
F	Measuring systems on pipelines and systems for loading ships
G	Measuring systems intended for the refuelling of aircraft
H*	<i>Self service arrangements with fuel dispensers</i>
I*	<i>Other self service arrangements</i>
J*	<i>Unattended delivery</i>
K*	<i>Measuring systems for bunker fuel (to be added later)</i>
L*	<i>Measuring systems for liquefied natural gas (LNG) (to be added later)</i>
X	Annex of a <u>A</u> dvice and S <u>S</u> uggested P <u>P</u> ractices

* ~~†~~†These Annexes are still under development (they are planned to be added at a later date – in a future revision of this ~~document~~Recommendation)

Dynamic ~~m~~Measuring ~~S~~systems for ~~L~~liquids other than ~~W~~water

Part 2: Metrological ~~c~~Controls and performance tests

1 Scope

1.1 This Recommendation specifies the metrological and technical requirements applicable to dynamic measuring systems for quantities (volume or mass) of liquids other than water subject to legal metrology controls. ~~It also provides requirements for the approval of specific components of the measuring systems (meter, electronic calculator, etc.).~~

1.2 In principle, this Recommendation applies to all measuring systems fitted with a meter as defined in T.m.3 (continuous measurement), whatever be the measuring principle of the meters or their application, ~~except:~~

- ~~D~~dynamic measuring devices and systems for cryogenic liquids (OIML R 81),
- ~~w~~Water meters for the metering of cold potable water and hot water (OIML R 49-1, ~~R-R~~ 49-2 and R 49-3),
- ~~h~~Heat meters (OIML R 75-1, R 75-2 and R 75-3).

1.3 This Recommendation is not intended to prevent the development of new technologies.

1.4 National or international regulations are expected to clearly specify which measuring systems for liquids other than water are subject to legal metrology controls. ~~For waste water measurement, it is up to the national authorities to decide whether the use of measuring systems conforming to this Recommendation is mandatory, and which accuracy class is required.~~

1.5 Part 2 of this Recommendation ~~—(R117R-117OIML R 117-2)~~ specifies the metrological controls and performance tests to meet the metrological and technical requirements of ~~R117R-117OIML R 117-1~~ for:

- the type evaluation of complete measuring systems, ~~and~~ and
- the type evaluation of constituent elements of a measuring system that are approved for separate type approval, ~~and~~ and

~~—the initial verification of complete measuring systems.~~

2 Metrological control

2.1 Type evaluation and approval

Measuring systems subject to legal metrology control shall be subject to type evaluation and approval.

In addition, the constituent elements of a measuring system, mainly those listed below, and the sub-systems which include several of these elements (for example, a flowcomputer), are able to receive separate type approval upon the request of the manufacturer:

meter;
measuring device;
meter sensor;
transducer;
calculator/electronic calculator;
indicating device;
gas separator;
gas extractor;
special gas extractor;
conversion device;
ancillary devices providing or memorizing measurements results:
printing device;
memory device;
self-service device;
temperature measuring device or sensor;
pressure measuring device or sensor;
density measuring device or sensor.

See also Annex X.2.1 (~~at the beginning of Annex X of R117 2~~) for the chart entitled on “General metrological requirements for specific components of a measuring system” ~~for a chart that which~~ shows the components that are able to receive a separate type approval cross-referenced with sections from ~~R117~~OIML R 117-1 that apply to each component.

Note: In some countries, the expressions “type evaluation” and “type approval” can be reserved for complete measuring systems. In this case, it is advisable that types of constituent elements be submitted to a procedure similar to type approval, making it possible to certify the conformity of the type of a constituent element to the regulation.

The constituent elements of a measuring system shall comply with the relevant requirements even when they have not been subject to separate type evaluation- (except in the case of ancillary devices and additional devices that are exempted from the controls).

Unless otherwise specified in this Recommendation, a measuring system shall fulfil the requirements without adjustment of the system or of its elements during the course of the tests. Relevant tests belonging together should be carried out on the same measuring system or element, under the same conditions and without adjustment. If, however, an adjustment has been performed or tests have been conducted with another measuring system and/or device this shall be documented and justified in the test report.

Any exceptions to the test procedures described in ~~R 117~~R 117OIML R 117-2 ~~must~~shall be fully and clearly documented in the type evaluation report.

2.2 Initial ~~y~~Verification

Measuring systems subject to legal metrology control shall be subject to initial verification.

The object of the initial verification is to verify the compliance of complete measuring systems with the requirements described in ~~R 117~~R 117OIML R 117-1, ~~Section~~ 6.2 and ensure the systems conforms to ~~its~~their approved type before ~~those systems~~they are place into service.

Test procedures for the initial verification of complete measuring systems are not yet complete;- when they are complete, these test procedures will be found in the individual annexes of this Recommendation.

Note ~~1~~: -Some of the draft initial verification test procedures for complete measuring systems can be found in Annex X (~~a~~Advice and suggested practices). Initial verification test procedures will be added in the immediate revision of all three parts of ~~R 117~~R 117OIML R 117.

~~—Temporary Note (2): a decision to not include initial verification test procedures in the Annexes of the 2CD of R 117-2 was made at a Project Group meeting in Teddington in October 2013. Instead, these test procedures are planned to be part of the next revision cycle.~~

3 Symbols, units and equations

In this Recommendation the following symbols, units and equations are used:-

CID	Calculator and indicating device
NCU	National currency unit
EUT	Equipment under test
MPE	Maximum permissible error
RH	Relative humidity
e	Scale interval (L, kg) of the main indicating device
f	Frequency of pulses sent to the CID (pulses per second)
i	Number of pulses sent to the CID
K	Variable determined by the ratio Q_{\min}/Q_{\max} and the number of flowrates for accuracy testing

$$K = \left[\frac{Q_{\min}}{Q_{\max}} \right]^{\frac{1}{N_F - 1}}$$

~~mmq~~MMQ Minimum measured quantity (L or kg --- see also V_{\min})

n_F Sequence number of a flowrate test

N_F Number of flowrates for accuracy testing

P_u Indicated unit price (NCU/L, NCU/kg)

p_t	Pressure of the liquid passing through the meter or the measurement transducer (bar)
p_{\min}	Minimum pressure of the liquid passing through the meter or the measurement transducer (bar)
p_{\max}	Maximum pressure of the liquid passing through the meter or the measurement transducer (bar)
μ	Dynamic viscosity of the liquid (mPa·s)
Q_s	Simulated flowrate of the liquid (L/min, kg/min)
Q	Flowrate of liquid (L/min, kg/min)
Q_{\min}	Minimum flowrate of liquid (L/min, kg/min)
Q_{\max}	Maximum flowrate of liquid (L/min, kg/min)
Q_a	Flowrate of air (L/min, kg/min)
t	Time (s)
T_s	Temperature of the liquid in the standard capacity measure (°C)
T_r	Reference temperature of the standard capacity measure (°C)
T_t	Temperature of the liquid passing through the meter or measurement transducer (°C)

U Expanded ~~U~~ncertainty

V_{\min}	Minimum measured quantity - volume (L)
V_i	Indicated volume at metering conditions by the CID (L)
V_s	Volume indication of the standard capacity measure (L)
V_r	Volume indication of the standard capacity measure, compensated from the deviation $Q = K^{n_F - 1} \times Q_{\max}$ of the reference temperature (L)
V_m	Volume at metering conditions stored by the CID if the CID is fitted with a memory device (L)
V_p	Printed volume at metering conditions if the CID is fitted with a printing device (L)
V_c	Volume at metering conditions calculated from the number of simulated pulses i and the k-factor k_f (L)
V_n	Volume at metering conditions (L) passing through the meter compensated for deviation from reference temperature of the standard capacity measure and pressure and temperature of the liquid
V_a	Volume of air (L)

M_i	Indicated mass CID (kg)
M_s	Mass indication of the weighing instrument (kg)

M_b	Mass indication of the weighing instrument, corrected for the buoyancy (kg)
M_m	Indicated mass stored by the CID if the CID is fitted with a memory device (kg)
M_p	Printed mass if the CID is fitted with a printing device (kg)
M_c	Mass calculated from the number of simulated pulses i and the k-factor k_f (kg)

k_f	k-factor, number of pulses per unit of quantity (pulses/L, pulses/kg)
α	Cubic expansion coefficient of the test liquid due to temperature ($^{\circ}\text{C}^{-1}$)
χ	Compressibility coefficient of the test liquid (bar^{-1})
β	Cubic expansion coefficient of the standard capacity measure due to temperature ($^{\circ}\text{C}^{-1}$)

Notes:- For the determination of α refer to OIML R 63 or ISO 91-1 for petroleum products.

For the determination of χ refer to [the](#) API Manual of Petroleum Measurements Standards Chapter 11.2.1 for petroleum products (new fuels issues, including E10)

-If β is not known, the following values can be used.

Material	$\beta(^{\circ}\text{C}^{-1})$ (uncertainty: $5 \times 10^{-6} \text{ }^{\circ}\text{C}^{-1}$)
Borosilica glass	10×10^{-6}
Glass	27×10^{-6}
Mild steel	33×10^{-6}
Stainless steel	51×10^{-6}
Copper, Brass	53×10^{-6}
Aluminium	69×10^{-6}

P_i	Indicated price (price to pay) by the CID (NCU)
P_m	Price stored by the CID if the CID is fitted with a memory device (NCU)
P_p	Printed price if the CID is fitted with a printing device (NCU)
P_c	Calculated price (NCU)
E_{vi}	Error of indicated volume at metering conditions (%)
E_{vm}	Error of stored volume at metering conditions if the CID is fitted with a memory device (%)
E_{vp}	Error of printed volume at metering conditions if the CID is fitted with a printing device (%)
E_{va}	Error of indicated volume at metering conditions resulting of the presence of air (%)
E_{mi}	Error of indicated mass (%)
E_{mm}	Error of stored mass if the CID is fitted with a memory device (%)
E_{mp}	Error of printed mass if the CID is fitted with a printing device (%)
E_{ma}	Error of indicated mass resulting of the presence of air (%)

ε_0	Intrinsic error of the instrument at metering conditions (%)
ε_1	Intrinsic error at metering conditions obtained at the first accuracy test (%)
ε_2	Intrinsic error at metering conditions obtained at the second accuracy test (%)
ε_3	Intrinsic error at metering conditions obtained at the third accuracy test (%)
$E_{vi}(B)$	Error of indicated volume at metering conditions before the endurance test (%)
$E_{vi}(A)$	Error of indicated volume at metering conditions after the endurance test (%)
$E_{mi}(B)$	Error of indicated mass, at metering conditions, before the endurance test (%)
$E_{mi}(A)$	Error of indicated mass, at metering conditions, conditions after the endurance test (%)
E_{pi}	Error of indicated price (NCU)
E_{pm}	Error of stored price if the CID is fitted with a memory device (NCU)
E_{pp}	Error of printed price if the CID is fitted with a printing device (NCU)
\bar{E}	Mean value of errors (% , NCU, °C, bar)
n	Number of tests at the same condition
Q_s	$= 60 \times i / (k_f \times t)$
V_c	$= i / k_f$
M_c	$= i / k_f$
P_c	$= V_i \times P_u, M_i \times P_u$
V_r	$= V_s [1 + \beta (T_s - T_r)]$
V_n	$= V_r [1 + \alpha(T_t - T_s)] \times [1 - \chi p_t]$

$$E_{vi} = [(V_i - V_c) / V_c] \times 100 \quad V_c \text{ may be replaced by } V_r \text{ or } V_{n-1} \text{ if appropriate}$$

$$E_{vm} = [(V_m - V_c) / V_c] \times 100 \quad V_c \text{ may be replaced by } V_r \text{ or } V_{n-1} \text{ if appropriate}$$

$$E_{vp} = [(V_p - V_c) / V_c] \times 100 \quad V_c \text{ may be replaced by } V_r \text{ or } V_{n-1} \text{ if appropriate}$$

$$E_{va} = [(V_i - V_c) / V_c] \times 100 \quad V_c \text{ may be replaced by } V_r \text{ or } V_{n-1} \text{ if appropriate}$$

$$E_{mi} = [(M_i - M_c) / M_c] \times 10 \quad V_c \text{ may be replaced by } M_b, \text{ if appropriate}$$

$$E_{mm} = [(M_m - M_c) / M_c] \times 100 \quad M_c \text{ may be replaced by } M_b, \text{ if appropriate}$$

$$E_{mp} = [(M_p - M_c) / M_c] \times 100 \quad M_c \text{ may be replaced by } M_b, \text{ if appropriate}$$

$$E_{ma} = [(M_i - M_c) / M_c] \times 100 \quad M_c \text{ may be replaced by } M_b, \text{ if appropriate}$$

$$E_{pi} = P_i - P_c$$

$$E_{pm} = P_m - P_c$$

$$E_{pp} = P_p - P_c$$

$$\bar{E} = [E(1) + E(2) + \dots + E(n)] / n$$

$$\varepsilon_{v1} = [(V_i - V_c) / V_{c1}] \times 100 \quad V_c \text{ may be replaced by } V_r \text{ or } V_{n-1} \text{ if appropriate}$$

$$\varepsilon_{v2} = [(V_i - V_c) / V_{c2}] \times 100 \quad V_c \text{ may be replaced by } V_r \text{ or } V_{n-1} \text{ if appropriate}$$

$$\varepsilon_{v3} = [(V_i - V_c) / V_{c3}] \times 100 \quad V_c \text{ may be replaced by } V_r \text{ or } V_{n-1} \text{ if appropriate}$$

$$\varepsilon_{m1} = [(M_i - M_c) / M_{c1}] \times 100 \quad M_c \text{ may be replaced by } M_b, \text{ if appropriate}$$

$$\varepsilon_{m2} = [(M_i - M_c) / M_{c2}] \times 100 \quad M_c \text{ may be replaced by } M_b, \text{ if appropriate}$$

$$\varepsilon_{m3} = [(M_i - M_c) / M_{c3}] \times 100 \quad M_c \text{ may be replaced by } M_b, \text{ if appropriate}$$

$$\varepsilon_0 = [\varepsilon_1 + \varepsilon_2 + \varepsilon_3] / 3$$

$$\text{Range} = \text{Maximum error} - \text{minimum error (\%, NCU)}$$

4 ~~Chapter~~, Type ~~E~~evaluation ~~P~~performance ~~T~~tests

4.1 General

This set of performance tests is intended to verify that the measuring system or its constituent elements operate as intended in a specified environment and under specified conditions. Each test indicates, where appropriate, the reference conditions for determining the intrinsic error.

Different kinds of tests are specified:

- ~~a~~Accuracy tests (including repeatability and flow disturbances tests, if applicable);
- ~~i~~Influence factor tests; and
- ~~D~~Disturbance tests.

~~The tests specified in this Recommendation are (considered to be sufficient) test procedures to meet the requirements of R 117-1. However, for new technologies or new applications, additional tests may be necessary to ensure compliance of the measuring system or its constituent elements with the requirements of this Recommendation.~~

~~The tests specified in this Recommendation constitute minimum (considered to be sufficient) test procedures to meet the requirements of R 117-1. Further tests may be undertaken, if necessary, to ensure compliance of the measuring system or its constituent elements with the requirements of this Recommendation.~~

When the effect of one influence quantity is being evaluated, all other influence quantities shall be held relatively constant, at values close to reference conditions.

More recent versions of the specific IEC and ISO standards referenced in this chapter's performance tests may be applied as long as the authority performing the type evaluation (the testing laboratory) confirms that the more recent versions continue to cover the testing requirements in this Recommendation.

Tests are ideally carried out on the complete measuring system, fitted with an indicating device, with all the ancillary devices, and with the correction device, if any. However, the meter subject to testing is not required to be fitted with its ancillary devices when the latter are not likely to influence the accuracy of the meter and when these have been verified separately (for example, an electronic printing device). The measuring device may also be tested separately provided that the calculator and the indicating device have been verified. The meter sensor may be tested separately provided that the transducer and the calculator with indicating device have been verified.

If this measuring device or meter sensor is intended to be connected to a calculator fitted with a correction device, the applicable correction algorithm(s) provided by the manufacturer shall be applied on the output signal of the transducer in order to determine its error.

4.2 ~~Measurement Uncertainty~~Uncertainties of measurement

~~4.1.14.2.1~~ -When a test is conducted, the expanded uncertainty of the determination of errors on indications of volume or mass shall be less than one-fifth of the maximum permissible error applicable for that test during type evaluation and one-third of the maximum permissible error applicable for that test during other verifications. The expanded uncertainty is calculated according to the “Guide to the expression of uncertainty in measurement” (2008 edition) with $k = 2$. ~~In the calculation of the uncertainty, the resolution of the EUT shall be taken into account.~~

~~4.1.24.2.2~~ -It is always preferable to apply ~~Section 4.2.1.~~ However, if it is technically or economically impractical to reach an uncertainty of 1/5 and 1/3 of the MPE, a “reduced $MPE = (6/5 \times MPE - U)$ ” and a “reduced $MPE = (4/3 \times MPE - U)$ ” respectively may be used. When calculating the expanded uncertainty, the resolution but not the repeatability of the EUT shall be included. This exception is only valid in the case of mutual agreement of the manufacturer and the test authority.— Use of this exception shall be fully documented.

~~**Note: It is planned that Section 4.2 will be moved into R117R 117-1 in the immediate revision of all three parts.**~~

4.3 ~~Note: This exception is only valid in mutual agreement of the manufacturer and the test facility, and only to approve a device. Use of this exception must be fully documented.~~Reference conditions

Ambient temperature:	15 °C to 35 °C
Relative humidity:	25 % to 75 %
Atmospheric pressure:	84 kPa to 106 kPa
Mains (power supply) voltage:	Nominal voltage (U_{nom})
Mains (power supply) frequency:	Nominal frequency (f_{nom})

During each test, the temperature shall not vary by more than 5 °C and the relative humidity shall not vary by more than 10 % within the reference range.

The test laboratory shall have the ability to authorize different reference conditions as long as these conditions are fully documented with an explanation of: why the alternate reference conditions were used, the implications of the alternate reference conditions, and the effects on the testing results.

4.4 ~~Test quantities~~volumes

Some influence quantities have a systematic (absolute) effect on measurement results and not a proportional effect related to the measured volume. If the fault limit is related to the measured volume (in order to be able to compare results obtained in different laboratories), it is necessary to perform a test on a fixed volume and ~~flow rate~~flowrate, and not less than the minimum measured quantity. Furthermore, the test volume shall be in accordance with the uncertainty requirements in ~~Section 4.2.~~

Note: -In this section, “fault limit” is the value that determines when a fault is a significant fault.

4.5 Preventing the liquid temperature ~~being from~~ being from influence ~~ing on~~ test results

Temperature tests concern testing the effect of the ambient temperature on the measurement result and not the effect of the temperature of the applied liquid. Simulation of the flow signal while performing the test is advisable in order to prevent the temperature of the liquid ~~being of from~~ being of from influence ~~ing to~~ the test results. – These test methods for evaluation ~~ing of the~~ ing of the influence of the ambient temperature are presented in ~~Section~~ Section 4.8.

FEDR

4.2

4.34.6 ~~Software setting / configuration~~

Software is a critical factor in the proper operation of an ~~measuring system~~electronic meter. Therefore, it must be verified that the software is configured correctly, and that the ~~t~~Type approval certificate includes any restriction in parameter setting/configuration.

Note:- This section needs addition consideration. The concept of this requirement will need to be repeated in the next revision of ~~R 117~~R-117OIML R 117-1 (~~Section~~6.1.2, etc.) and space for the software settings/configurations/parameters will included in the ~~R 117~~R-117OIML R 117-3 “~~F~~Format of the test report”.

4.44.7 Reverse flow (from ~~R 117~~R-117OIML R 117-1, ~~Section~~2.13.4)

Check if a reversal of the flow results in an error greater than the minimum specified quantity deviation. -If so, the measuring system (in which the liquid could flow in the opposite direction) shall be provided with a non-return valve. See also flow computers section.

Note 1:- See ~~Section~~5 for “Testing procedures for meter sensors and measuring devices”.

Note 2:- See ~~Section~~6 for “Testing procedures for electronic calculators (that may be equipped with a conversion device), indicating devices and associated devices”.

4.8 Disturbance and iInfluence Ffactor Ttests - climatic and mechanical environmental conditions

4.8.1 General

The general reference for testing requirements in 4.8 is OIML D 11:2013.

The test procedures in 4.8 have been given in condensed form, for information only, and are adapted from the referenced IEC and ISO publications. Before conducting the tests, the applicable publications should be consulted.

4.8.1.1 For each performance test, typical test conditions are indicated; these conditions correspond to the climatic and mechanical environmental conditions to which measuring systems are usually exposed.

4.8.1.2 -The applicant for type evaluation shall specify the rated operating conditions and the specific environmental conditions in the documentation supplied to the authority performing the type evaluation (the testing laboratory) based on the intended use of the instrument. Higher severity levels may be requested by the manufacturer. -The authority performing the type evaluation (the testing laboratory) shall conduct performance tests at the agreed severity levels. If type approval is granted, the data plate on the EUT shall indicate the corresponding limits of use. Manufacturers shall inform potential users of the environmental conditions for which the instrument is approved. The authority performing the type evaluation (the testing laboratory) shall verify that these environmental conditions are met.

4.8.2 Test levels for temperature

The thermal conditions in which measuring systems and ancillary devices are used vary considerably. These ~~are do~~ not only highly dependent on the place on earth, ranging from arctic to tropical regions, but are also considerably dependent on indoor or outdoor applications. Devices ~~being~~ typically used

indoors in one country can be typically used outdoors in other countries. Therefore, no classes combining low and high temperature limits have been described in this Recommendation.

Note:- While manufacturers select the test levels for type evaluation, national (or regional) legislation will generally set the requirements for acceptable lower and upper temperature limits (taking into account the test levels in 4.8.5 and 4.8.6.).

4.8.3 Classification for humidity

The following table gives a classification for the test levels (severity levels) for the humidity tests:

Class	Test level Damp heat (cyclic)	Description
H1	-	<p>This class applies to instruments or parts of instruments typically used in temperature-controlled enclosed (weather-protected) locations. Where necessary, heating, cooling or humidification is used to maintain the required environmental conditions. Measuring instruments are not exposed to condensed water, precipitation, or ice formations.</p> <p>These conditions may apply in living areas, continuously staffed offices, certain workshops, and other rooms for special applications.</p>
H2	1	<p>This class applies to instruments or parts of instruments typically used in enclosed (weather-protected) locations where the local climate is not controlled. Measuring instruments present may be subject to condensed water, water from sources other than rain, and to ice formations.</p> <p>These conditions may apply in some publicly-accessible areas in buildings, garages, below-ground areas, certain workshops, factories, industrial plants, ordinary storage rooms for frost-resistant products, farm buildings, etc.</p>
H3	2	<p>This class applies to instruments or parts of instruments used in open air locations excluding those in extreme climate zones such as polar and desert environments.</p>

4.8.4 Classification for mechanical tests

The following table gives a classification for the test levels (severity levels) for mechanical tests:

Class	Test level Vibration	Description
M1	-	<p>This class applies to locations with vibration of low significance</p> <p>For example, for instruments fastened to light supporting structures subject to negligible vibrations and shocks (transmitted from local blasting or pile-driving activities, slamming doors, etc.)</p>
M2	1	<p>This class applies to locations with significant or high levels of vibration and shock</p> <p>For example, vibration and shock transmitted from machines and passing vehicles in the vicinity or adjacent to heavy machines, conveyor belts, etc.</p>
M3	2	<p>This class applies to locations where the level of vibration is high and/or very high</p> <p>For example, for measuring instruments mounted directly on machines, conveyor belts, etc.</p>

Table 4.8.5 Dry heat

Applicable standards	IEC 60068-2-2 [12], IEC 60068-3-1 [16]					
Test method	Exposure to dry heat (non-condensing)					
Applicability	General					
Object of the test	Verification of compliance with the provisions in R-117 <u>QIML R 117-1</u> , <u>Section 4.1.1</u> under conditions of high temperature					
Test procedure in brief	<p>The test comprises exposure to the specified high temperature under “free air” conditions during the period of time specified (the period specified is the period succeeding the moment at which the EUT has reached temperature stability).</p> <p>The change in temperature shall not exceed 1 °C/min during heating up and cooling down.</p> <p>The absolute humidity of the test atmosphere shall not exceed 20 g/m³.</p> <p>When tests are performed at temperatures below 35 °C, the relative humidity shall not exceed 50 %.</p> <p>The EUT shall be tested:</p> <ul style="list-style-type: none"> at the reference temperature of 20 °C after 1 hour conditioning; at the specified high temperature, 2 hours after temperature stabilization; <ul style="list-style-type: none"> after 1 hour recovery of the EUT at the reference temperature of 20 °C. <p>During tests, the <u>During the tests, the</u> EUT shall be in operation. Simulated inputs are permitted. Tests shall be performed at a minimum of one flow rate <u>flowrate</u></p>					
	One of the following test levels may be specified:					
Test level index	1	2	3	4	5	unit
Temperature	30	40	55	70	85	°C
Duration	2	2	2	2	2	hours
Permitted maximum deviation	All functions shall operate as designed. All errors shall be within the maximum permissible errors.					

Table 4.8.6 Cold

Applicable standards	IEC 60068-2-1 [11], IEC 60068-3-1 [16]				
Test method	Exposure to low temperature				
Applicability	General				
Object of the test	Verification of compliance with the provisions in R 117 <u>QIML R 117-1</u> , <u>Section 4.1.1</u> under conditions of low temperature				
Test procedure in brief	<p>The test comprises exposure to the specified low temperature under “free air” conditions for a 2-hour period after the EUT has reached temperature stability.</p> <p>The change of temperature shall not exceed 1 °C/min during heating up and cooling down.</p> <p>IEC specifies that the power to the EUT shall be switched off before the temperature is raised.</p> <p>The EUT shall be tested:</p> <ul style="list-style-type: none"> at the reference temperature of 20 °C after 1 hour conditioning, at the specified low temperature, 2 hours after temperature stabilization, after 1 hour recovery of the EUT at the reference temperature of 20 °C. <p>During tests, the <u>During the tests, the</u> EUT shall be in operation. Simulated inputs are permitted. Tests shall be performed at a minimum of one flow rate <u>flowrate</u></p>				
	One of the following test levels may be specified:				
Test level index	1	2	3	4	unit
Temperature	+5	-10	-25	-40	°C
Duration	2	2	2	2	hours
Permitted maximum deviation	All functions shall operate as designed. All errors shall be within the maximum permissible errors.				

Table 4.8.7 Damp heat, cyclic (condensing)

Applicable standards	IEC 60068-2-30 [13], IEC 60068-3-4 [17]		
Test method	Exposure to damp heat with- cyclic temperature variation		
Applicability	Applicable only for outdoor used equipment		
Object of the test	Verification of compliance with the provisions in R-117 OIML R 117-1, 4.1.1 under conditions of high humidity combined with cyclic temperature changes		
Test procedure in brief	<p>The test comprises exposure to cyclic temperature variation between 25 °C and the appropriate upper temperature while maintaining the relative humidity above 95 % during the temperature change and the low temperature phases and at or above 93 % RH at the upper temperature phases.</p> <p>Condensation is expected to occur on the EUT during the temperature rise.</p> <p>The 24-hour cycle comprises:</p> <ol style="list-style-type: none"> 1) temperature rise during 3 hours, 2) temperature maintained at upper value until 12 hours from the start of the cycle, 3) temperature lowered to lower temperature level- within a period of 3 to 6 hours, the declination (rate of fall) during the first hour and a half being such that the lower temperature level would be reached in a 3 hours period, 4) temperature maintained at the lower level until the 24 h period is completed. <p>The stabilizing period before and recovery period after the cyclic exposure shall be such that the temperature of all parts of the EUT is within 3 °C of its final value.</p> <p>Special electrical conditions and recovery conditions may need to be specified.</p> <p>For integrating measuring instrument see R-117OIML R 117-1, Section sub-clause9.2.2 for the appropriate sequence of measurements during- the test.</p> <p>During tests, theDuring the tests, the EUT shall be in operation. Simulated inputs are permitted. After the application of the disturbance influence factor and recovery the EUT shall be tested at a minimum of one flow rateflowrate.</p>		
	One of the following test levels may be specified:		
Test level index	1	2	unit
Upper temperature	40	55	°C
Duration	2	2	24-hour cycle
Restrictions	During the application of the disturbance, influence quantity the power supply of the EUT is in switch-off mode.		
Permitted maximum deviation	After the application of the disturbanceinfluence factor and recovery: All functions shall operate as designed. All errors shall be within the		

	maximum permissible errors.
--	-----------------------------

FEDOR

Table 4.8.8 Vibration (random)

Applicable standard	IEC 60068-2-47 [14], IEC 60068-2-64 [15], (IEC 60068-3-8 [xx])		
Test method	Exposure to random vibration		
Applicability	General		
Object of the test	Verification of compliance with the provisions in R-117 OIML R 117-1, Section 4.1.1 under conditions of random vibration		
Test procedure in brief	<p>The test comprises exposure of the EUT to vibration.</p> <p>The EUT shall be tested in three, mutually perpendicular axes mounted on a rigid fixture by its normal mounting means.</p> <p>The EUT shall normally be mounted in such a way that the gravity vector points in the same direction as it would in normal use. Where on basis of the measurement principle the direction the effect can be assumed negligible the EUT may be mounted in any position.</p> <p>After the application of the influence factor, the EUT shall be tested at a minimum of one flow-rateflowrate.</p>		
	One of the following test levels may be specified:		
Test level index	1	2	unit
Total frequency range	10 – 150	10 – 150	Hz
Total RMS level	1.6	7	m·s ⁻²
ASD level 10-20 Hz	0.05	1	m ² ·s ⁻³
ASD level 20-150 Hz	-3	-3	dB/octave
Duration per axis	For each of the orthogonal directions the vibration exposure time shall be 2 minutes.		
Restrictions	During the application of the influence quantity the power supply of the EUT is in switch-off mode.		
Permitted maximum deviation	After the influence factor is removed: all functions shall operate as designed. All errors shall be within the maximum permissible errors.		

4.9 Disturbance ~~and Influence Factor Tests~~ – electrical tests

4.9.1 General

The general reference for testing requirements in ~~R-117~~OIML R 117-1, ~~Sections~~ 4.9 and 4.10 is OIML D 11:2013. Test procedures in 4.9 and 4.10 have been given in condensed form, for information only, and are adapted from the referenced IEC publications. Before conducting the tests, the applicable publications should be consulted.

4.9.1.1 –Severity levels for electrical disturbance tests

The following table gives a classification for electrical disturbance tests:

Class	Description
E1	This class applies to measuring instruments used in locations where electromagnetic disturbances correspond to those likely to be found in a residential, commercial and/or light industrial environments.
E2	This class applies to measuring instruments used in locations where electromagnetic disturbances correspond to those likely to be found in industrial buildings.
E3	This class applies to measuring instruments powered by the battery of a vehicle and exposed to electromagnetic disturbances which correspond to those likely to be found in any environment not generally considered hazardous for the general public.

The relation between the class and the applicable test levels (severity levels) is given in the following table.

Test level (Severity level) for class			Test			
E1	E2	E3	R-117 OIML R 117-2 Section	Test Description	Evaluation	
1	1	--	4.9.2.1	AC mains voltage variation	I	MPE
--	--	--	4.9.2.2	DC mains voltage variation	I	MPE
1	2	--	4.9.3	AC mains power – voltage dips, short interruptions, and voltage variations	D	NSFd
2	3	--	4.9.4	Bursts (transients) on AC and DC mains	D	NSFd
3	3	3	4.9.5	Electrostatic discharge (ESD)	D	NSFa (1) NSFd (2)
2	3	--	4.9.6	Bursts (transients) on signal, data and control lines	D	NSFd
3	3	--	4.9.7	Surges on signal, data and control lines	D	NSFa (1) NSFd (2)
--	1	--	4.9.8	DC mains power – voltage dips, short interruptions and voltage variations	D	NSFa (1) NSFd (2)
--	1	--	4.9.9	Ripple on DC input power ports	D	NSFd
3	3	--	4.9.10	Surges on AC and DC mains lines	D	NSFa
2	3	3	4.9.11.1	Radiated radio frequency electromagnetic fields of general origin	D	NSFd
3	3	3	4.9.11.2	Radiated radio frequency electromagnetic fields (digital radio telephones)	D	NSFd
2	3	3	4.9.11.3	Conducted (common mode) currents generated by radio frequency electromagnetic fields	D	NSFd
--	--	C or F	4.10.1	Voltage variations (road vehicle battery)	I	MPE
--	--	IV	4.10.2	Electrical transient conduction along supply lines (EUT powered by road vehicle battery)	D	NSFd
--	--	I + III	4.10.3	Battery voltage variations during starting up a vehicle engine	D	NSFa (1) NSFd (2)
--	--	I + II	4.10.4	Load dump test	D	NSFa

Guide:

I = Influence factor

D = Disturbance

MPE = Maximum permissible error ~~according to 3.6~~

NSFa = No significant fault shall occur after the disturbance

NSFd = No significant fault shall occur during the disturbance

(1) For integrating instruments (~~analogue~~analog)

(2) For non-integrating instruments (digital)

~~The relation between the class and the applicable test levels (severity levels) is given in the following table.~~

Test Level (Severity Level) for class			Test	
E1	E2	E3	R-117 OIML R 117-2 Section	Test Description
1	1	—	4.9.2.1	AC mains voltage variation
—	—	—	4.9.2.2	DC mains voltage variation
1	2	—	4.9.3	AC mains power — voltage dips, short interruptions, and voltage variations
2	3	—	4.9.4	Bursts (transients) on AC and DC mains
3	3	3	4.9.5	Electrostatic discharge (ESD)
2	3	—	4.9.6	Bursts (transients) on signal, data and control lines
3	3	—	4.9.7	Surges on signal, data and control lines
—	1	—	4.9.8	DC mains power — voltage dips, short interruptions and voltage variations
—	1	—	4.9.9	Ripple on DC input power ports
3	3	—	4.9.10	Surges on AC and DC mains lines
2	3	3	4.9.11.1	Radiated radio frequency electromagnetic fields of general origin
3	3	3	4.9.11.2	Radiated radio frequency electromagnetic fields (digital radio telephones)
2	3	3	4.9.11.3	Conducted (common mode) currents generated by radio frequency electromagnetic fields

—	—	C or F	4.10.1	Voltage variations (road vehicle battery)
—	—	IV	4.10.2	Electrical transient conduction along supply lines (EUT powered by road vehicle battery)
—	—	I + III	4.10.3	Battery voltage variations during starting up a vehicle engine
—	—	I + II	4.10.4	Load dump test

4.4.1.14.9.1.2 —Electronic devices powered by batteries

There is a distinction between the tests for instruments powered by:

- a) ~~D~~isposable batteries;
- b) ~~g~~General rechargeable batteries; and
- c) ~~b~~Batteries of road vehicles.

For the case of disposable and rechargeable batteries of a general nature, no standards concerning the response instruments to the battery condition are available.

Devices powered by non-rechargeable batteries or by rechargeable batteries that cannot be (re)charged during the operation of the measuring system, shall comply with the following requirements:

- a) The device provided with new or fully charged batteries of the specified type shall comply with the applicable metrological requirements;
- b) As soon as the battery voltage has dropped to a value specified by the manufacturer as the minimum value of voltage ~~where-at which~~ the device complies with metrological requirements, this shall be detected and acted upon by the device in accordance with ~~Section 4.2 of R-117~~OIML R 117-1, 4.2.

For these devices, no special tests for disturbances associated with the ~~“m-mains”~~ power have to be carried out.

Devices powered by rechargeable auxiliary batteries that are intended to be (re)charged during the operation of the measuring instrument shall both:

- a) comply with the requirements for devices powered by non-rechargeable batteries or by rechargeable batteries that cannot be (re)charged during the operation of the measuring system, with the mains power switched off; and
- b) comply with the requirements for AC mains powered devices with the mains power switched on.

Devices powered by mains power and provided with a back-up battery for data-storage only, shall comply with the requirements for AC mains powered devices.

For electronic devices powered by the on-board battery of a road vehicle, a series of special tests for disturbances associated with the power supply are given in 4.10.

Table 4.9.2.1 AC mains voltage variation

Applicable standards		IEC/TR3 61000-2-1 [18], IEC 61000-4-1 [20]
Test method		Applying low and high level AC mains power voltage (single phase)
Applicability		Only applicable for measuring instruments which are temporarily or permanently connected to an AC mains power network while in operation This test is not applicable to equipment powered by a road vehicle battery.
Object of the test		Verification of compliance with the provisions in R-117 OIML R 117-1, Section 4.1.1 under conditions of AC mains network voltage changes between upper and lower limits
Test procedure in brief		The test comprises exposure of the EUT to the lower and upper limit power supply condition for a period sufficient for achieving temperature stability and subsequently performing the required measurements <u>while the EUT is operating under normal atmospheric conditions.</u> while the EUT is operating under normal atmospheric conditions. During tests, the During the tests, the EUT shall be in operation. Simulated inputs are permitted. Tests shall be performed at a minimum of one flow rate flowrate.
Test level		The following test levels are applicable:
Mains voltage	Upper limit	$U_{nom1} + 10 \%$
	Lower limit	$U_{nom2} - 15 \%$
		The values of U_{nom} are those as specified by the manufacturer and marked on the measuring instrument. In the case a range is specified U_{nom1} concerns the highest and U_{nom2} concerns the lowest value of that range. If only one nominal mains voltage value (U_{nom}) is presented then $U_{nom1} = U_{nom2} = U_{nom}$.
Extend		In the case of three phase power supply, the voltage variation shall apply for each phase successively.
Permitted maximum deviation		At supply voltage levels between upper and lower limit: <ul style="list-style-type: none"> all functions shall operate as designed. all errors shall be within the maximum permissible errors.

Table 4.9.2.2 DC mains voltage variation

Applicable standard	IEC 60654-2 [19]
Test method	Applying low and high level DC mains power voltage.
Applicability	Only applicable for measuring instruments which are temporarily or permanently connected to a DC mains power network while in operation and generally only applicable in industrial environment. (see sub-clause 8.4.1 of D 11). This test is not applicable to equipment powered by a road vehicle battery.
Object of the test	Verification of compliance with the provisions in R-117 OIML R 117-1, Section 4.1.1 under conditions of DC mains power voltage changes between upper and lower limit.
Test procedure in brief	<p>The test comprises exposure to the specified power supply condition for a period sufficient for achieving temperature stability and subsequently performing the required measurements.</p> <p>The test consists of exposure of the EUT to the specified power supply conditions while the EUT is operating under normal atmospheric conditions.</p> <p>During tests, theDuring the tests, the EUT shall be in operation. Simulated inputs are permitted. Tests shall be performed at a minimum of one flow-rateflowrate.</p>
Test level	<p>The upper voltage limit is the DC level at which the EUT has been manufactured to automatically detect high-level conditions.</p> <p>The lower limit will be the DC level at which the EUT has been manufactured to automatically detect low-level conditions.</p> <p>The EUT shall comply with the specified maximum permissible errors at voltage levels between the two levels. Testing may be restricted to subsequent exposure to the upper and lower voltage levels.</p>
Restrictions	<p>The DC operating range as specified by the manufacturer but not less than</p> $U_{nom} - 15 \% \leq U_{nom} \leq U_{nom} + 10 \%$
Permitted maximum deviation	<p>At supply voltage levels between upper and lower limit:</p> <p>All functions shall operate as designed.</p> <p>All errors shall be within the maximum permissible errors.</p>

Table 4.9.3 AC mains voltage dips, short interruptions and reductions

Applicable standards		IEC 61000-4-11 [26], IEC 61000-6-1 [29], IEC 61000-6-2 [30]			
Test method		Introducing short-time reductions of mains voltage using the test set-up <u>setup</u> defined in the applicable standard			
Applicability		Only applicable for measuring instruments with rated input current of less than 16 A per phase which are temporarily or permanently connected to an AC mains power network while in operation. – This test is only applicable to equipment powered by AC mains supply and is not applicable to equipment powered by a road vehicle battery.			
Object of the test		Verification of compliance with the provisions in R-117 <u>QIML R 117-1, Section 4.1.1</u> under conditions of short time mains voltage reductions.			
Test procedure in brief		A test generator is to be used which is suitable to reduce the amplitude of the AC mains voltage for the required period of time. The performance of the test generator shall be verified before connecting the EUT. The mains voltage reduction tests shall be repeated 10 times with intervals of at least 10 s between the tests. The tests shall be applied continuously during the measurement time. The interruptions and reductions are repeated throughout the time necessary to perform the whole test; for this reason, more than ten interruptions and reductions may be necessary. During tests, the <u>During the tests, the</u> EUT shall be in operation. Simulated inputs are permitted. Tests shall be performed at a minimum of one flow rate <u>flowrate</u> .			
		One of the following test levels may be specified:			
Test level index			1	2	unit
Voltage dips	Test a	Reduction to	0	0	%
		Duration	0.5	0.5	cycles
	Test b	Reduction to	0	0	%
		Duration	1	1	cycles
	Test c	Reduction to	70	40	%
		Duration	25/30	10/12	cycles
	Test d	Reduction to	n/a	70	%
		Duration	n/a	25/30	cycles
	Test e	Reduction to	n/a	80	%
		Duration	n/a	250/300	cycles
Permitted maximum deviation		a) E <u>for</u> interruptible measuring systems: either significant faults do not occur or checking facilities detect a malfunctioning and act upon in it accordance <u>upon it in accordance</u> with 4.3 when significant faults occur.			

	b) F for non-interruptible measuring systems: no significant faults occur.
--	---

Table 4.9.4 Bursts (transients) on AC and DC mains

Applicable standards	IEC 61000-4-4 [23]		
Test method	Introducing transients on the mains power lines		
Applicability	<p>Only applicable for electronic measuring instruments which are temporarily or permanently connected to a mains power network while in operation.</p> <p>This test is not applicable to instruments connected to road vehicle batteries; see A.12 for specific testing requirements on these instruments.</p>		
Object of the test	Verification of compliance with the provisions in R-117 OIML R 117-1, Section 4.1.1 during conditions where electrical bursts are superimposed on the mains voltage.		
Test procedure in brief	<p>A burst generator as defined in the referred standard shall be used.</p> <p>The characteristics of the generator shall be verified before connecting the EUT.</p> <p>The test comprises exposure to bursts of voltage spikes for which the output voltage on 50 Ω and 1000 Ω load are defined in the referred standard.</p> <p>Both positive and negative polarity of the bursts shall be applied.</p> <p>The duration of the test shall not be less than 1 min for each amplitude and polarity. The injection network on the mains shall contain blocking filters to prevent the burst energy being dissipated in the mains.</p> <p>At least 10 positive and negative randomly phased bursts shall be applied.</p> <p>The bursts are applied during all the time necessary to perform the test; therefore, more bursts than indicated above may be necessary.</p> <p>During tests, theDuring the tests, the EUT shall be in operation. Simulated inputs are permitted. Tests shall be performed at a minimum of one flow rateflowrate.</p>		
	One of the following test levels may be specified:		
Test level index	2	3	unit
Amplitude (peak value)	1	2	kV
Repetition rate	5	5	kHz
Permitted maximum deviation	<p>a) Ffor interruptible measuring systems: either significant faults do not occur or checking facilities detect a malfunctioning and act upon in it accordance upon it in accordance with R-117OIML R 117-1, Section 4.3 when significant faults occur.</p> <p>b) fEfor non-interruptible measuring systems: no significant faults occur.</p>		

FEDOR

Table 4.9.5 Electrostatic discharge

Applicable standard	IEC 61000-4-2 [21]		
Test method	Exposure to electrostatic discharge (ESD)		
Applicability	Applicable to all electronic measuring instruments		
Object of the test	Verification of compliance with the provisions in R-117 OIML R 117-1, Section 4.1.1 in case of direct exposure to electrostatic discharges or such discharges in the neighbourhood of the EUT.		
Test procedure in brief	<p>The test comprises exposure of the EUT to electrical discharges.</p> <p>An ESD generator as defined in the referred standard shall be used and the test set-upsetup shall comply with the dimensions, materials used and conditions as specified in the referred standard. Before starting the tests, the performance of the generator shall be verified.</p> <p>At least 10 discharges per preselected discharge location shall be applied. For EUTs not equipped with a ground terminal, the EUT shall be fully discharged between discharges. The time interval between successive discharges shall be at least 1 second.</p> <p>Contact discharge is the preferred test method. Air discharge is far less defined and reproducible and therefore shall be used only where contact discharge cannot be applied.</p> <p>Direct application: In the contact discharge mode to be carried out on conductive surfaces, the electrode shall be in contact with the EUT before activation of the discharge. In such <u>a</u> case the discharge spark occurs in the vacuum relays of the contact discharge tip.</p> <p>On insulated surfaces only the air discharge mode can be applied. The EUT is approached by the charged electrode until a spark discharge occurs.</p> <p>During tests, theDuring the tests, the EUT shall be in operation. Simulated inputs are permitted. Tests shall be performed at a minimum of one flow-rateflowrate.</p>		
Test level index		3	unit
Test voltage	Contact discharge	6	kV
	Air discharge	8	kV
Permitted maximum deviation	<p>a) fFor interruptible measuring systems: either significant faults do not occur or checking facilities detect a malfunctioning and act upon in-it <u>in</u> accordance with R-117OIML R 117-1, Section 4.3 when significant faults occur.</p> <p>b) fFor non-interruptible measuring systems: no significant faults occur.</p>		

Table 4.9.6 Bursts (transients) on signal, data and control lines

Applicable standards	IEC 61000-4-4 [23]		
Test method	Introducing transients on signal, data and control lines		
Applicability	<p>Only applicable for electronic measuring instruments containing active electronic circuits which during operation are permanently or temporarily connected to external electrical signal, data and/or control lines.</p> <p>This test is not applicable to equipment powered by a road vehicle battery.</p>		
Object of the test	Verification of compliance with the provisions in R-117 <u>QIML R 117-1, Section 4.1.1</u> during conditions where electrical bursts are superimposed on I/O and communication ports.		
Test procedure in brief	<p>A burst generator as defined in the referred standard shall be used. The characteristics of the generator shall be verified before connecting the EUT.</p> <p>The test comprises exposure to bursts of voltage spikes for which the output voltage on <u>50 Ω and 1000 Ω</u> 50 W and 1000 W load are defined in the referred standard.</p> <p>Both positive and negative polarity of the bursts shall be applied.</p> <p>The duration of the test shall not be less than 1 min for each amplitude and polarity.</p> <p>A capacitive coupling clamp as defined in the standard shall be used for the coupling of the bursts into the I/O and communication lines.</p> <p>The bursts are applied during all the time necessary to perform the test; for that purpose more bursts than indicated above may be necessary.</p> <p>During <u>the</u> tests, the EUT shall be in operation. Simulated inputs are permitted. Tests shall be performed at a minimum of one flow <u>rate</u> flowrate.</p>		
	One of the following test levels may be specified:		
Test level index	2	3	unit
Amplitude (peak value)	0.5	1	kV
Repetition rate	5	5	kHz
Restrictions	Tests on signal lines are applicable only for I/O signal, data and control ports, with a cable length exceeding 3 m (as specified by the manufacturer).		
Permitted maximum deviation	<p>a) Ffor interruptible measuring systems: either significant faults do not occur or checking facilities detect a malfunctioning and act upon in it accordance upon it in accordance with R-117 <u>QIML R 117-1, Section 4.3</u> when significant faults occur.</p> <p>b) Ffor non-interruptible measuring systems: no significant faults occur.</p> <p>In either a) or b) above, human intervention is permitted to put the</p>		

	EUT into operation after the test (e.g. replacing a fuse), provided that all relevant data is available after the human intervention.
--	---

Table 4.9.7 Surges on signal, data and control lines

Applicable standard	IEC 61000-4-5 [24]			
Test method	Introducing electrical surges on signal, data and control lines			
Applicability	Only applicable for electronic measuring instruments containing active electronic circuits which during operation are temporarily or permanently connected to electrical signal, data and/or control lines that may exceed a length of 10 m. This test is not applicable to equipment powered by a road vehicle battery.			
Object of the test	Verification of compliance with the provisions in R-117 <u>R-117</u> OIML R 117-1, Section 4.1.1 during conditions where electrical surges are superimposed on I/O and communication ports.			
Test procedure in brief	<p>A surge generator as defined in the referred standard shall be used. The characteristics of the generator shall be verified before connecting the EUT.</p> <p>The test comprises exposure to electrical surges for which the rise time, pulse width, peak values of the output voltage/current on high/low impedance load and the minimum time interval between two successive pulses are defined in the referred standard.</p> <p>At least 3 positive and 3 negative surges shall be applied. The applicable injection network depends on the kind of wiring the surge is coupled into and is defined in the referred standard.</p> <p>The surges are applied during all the time necessary to perform the test; to that purpose more surges than indicated above may be necessary.</p> <p>During tests, the<u>During the tests, the</u> EUT shall be in operation. Simulated inputs are permitted. Tests shall be performed at a minimum of one flow rate<u>flowrate</u>.</p>			
	One of the following test levels may be specified:			
Test level index (installation class)			3	unit
	Unsymmetrical lines	Line to line	1.0	kV
		Line(s) to ground	2.0	kV
	Symmetrical lines	Line(s) to ground	2.0	kV
	Shielded I/O and communication lines		2.0	kV
Restrictions	1. Test on signal lines applies <u>only</u> for I/O, signal, data and control ports, with a cable length exceeding 30 m (as specified by the manufacturer). 2. Indoor DC signal, data, and control cables (regardless of length) are exempt from this test.			
Permitted maximum deviation	<p>a) F<u>For</u> interruptible measuring systems: either significant faults do not occur or checking facilities detect a malfunctioning and act upon in it accordance<u>upon it in accordance</u> with R-117<u>R-117</u>OIML R 117-1, Section 4.3 when significant faults occur.</p> <p>b) For non-interruptible measuring systems: no significant faults occur.</p>			

	In either a) or b) above, human intervention is permitted to put the EUT into operation after the test (e.g. replacing a fuse), provided that all relevant data is available after the human intervention.
--	--

Table 4.9.8 DC mains voltage dips, short interruptions and (short term) variations

Applicable standard		IEC 61000-4-29 [28]; IEC 61000-4-1	
Test method		Introducing voltage dips, short interruptions and voltage variations on DC mains power lines using the test set-up <u>setup</u> defined in the applicable standard	
Applicability		Only applicable for measuring instruments which are temporarily or permanently connected to a DC mains power network while in operation. This test is only applicable to equipment powered by DC mains supply and is not applicable to equipment powered by a road vehicle battery.	
Object of the test		Verification of compliance with the provisions in R117R-117 <u>QIML R 117-1, Section 4.1.1</u> under conditions of voltage dips, voltage variations and short interruptions on DC mains.	
Test procedure in brief		<p>A test generator as defined in the referred standard shall be used. Before starting the tests, the performance of the generator shall be verified.</p> <p>The EUT shall be exposed to voltage dips, short interruptions, for each of the selected combinations of amplitude and duration, using a sequence of three dips/interruptions and intervals of at least 10 s between each test event.</p> <p>The most representative operating modes of the EUT shall be tested three times at 10 s intervals for each of the specified voltage variations.</p> <p>If the EUT is an integrating instrument, the test pulses shall be continuously applied during the measurement time.</p> <p>The disturbances are applied during all the time necessary to perform the test; to that purpose more disturbances than indicated above may be necessary.</p> <p>During <u>the</u> tests, the EUT shall be in operation. Simulated inputs are permitted. Tests shall be performed at a minimum of one flow-rate <u>flowrate</u>.</p>	
Voltage dips			unit
	Amplitude	40 and 70	% of the rated voltage
	Duration	0.01; 0.03; 0.1; 0.3; 1; t	s
Short interruptions	Test condition	High impedance and/or low impedance	
	Amplitude	0	% of the rated voltage
	Duration	0.001; 0.003; 0.01; 0.03; 0.1; 0.3; 1; t	s
Voltage variations	Amplitude	85 and 120	% of the rated voltage
	Duration	0.1; 0.3; 1; 3; 10; t	s
Restrictions		If the EUT is tested for short interruptions, it is unnecessary to test for other levels of the same duration, unless the immunity of the equipment is detrimentally affected by voltage dips of less than 70 % of the rated voltage.	
Permitted maximum deviation		<p>a) fFor interruptible measuring systems: either significant faults do not occur or checking facilities detect a malfunctioning and act upon it <u>in accordance with</u> R117R-117 <u>QIML R 117-1</u>.</p>	

	<p>Section 4.3 when significant faults occur.</p> <p>b) Ffor non-interruptible measuring systems: no significant faults occur.</p>
--	---

EDR

Table 4.9.9 Ripple on DC mains power

Applicable standard	IEC 61000-4-17 [27] and IEC 6100-4-1	
Test method	Introducing a ripple voltage on the DC input power port.	
Applicability	<p>Only applicable for measuring instruments which are temporarily or permanently connected to a DC mains power network (distribution system) supplied by external rectifier systems while in operation and generally only applicable in <u>an industrial environment</u>. (see <u>OIML sub-clause 8.4.1 of D-11, 8.4.1</u>).</p> <p>This test is only applicable to equipment powered by DC mains supply and is not applicable to equipment powered by a road vehicle battery.</p>	
Object of the test	Verification of compliance with the provisions in R-117 OIML R 117-1, <u>Section 4.1.1</u> under conditions of the introduction of a ripple on the DC mains voltage. This test is not applicable for instruments connected to battery charger systems with incorporated switch mode converters.	
Test procedure in brief	<p>A test generator as defined in the referred standard shall be used. Before starting the tests, the performance of the generator shall be verified.</p> <p>The test comprises subjecting the EUT to ripple voltages such as those generated by traditional rectifier systems and/or auxiliary service battery chargers overlaying on DC power supply sources.</p> <p>The frequency of the ripple voltage is the applicable power frequency or a multiple (2, 3 or 6) dependant on the rectifier system used for the mains- <u>(as specified in the product specification)</u>.</p> <p>The waveform of the ripple, at the output of the test generator, has a sinusoid-linear character.</p> <p>The test shall be applied for at least 10 min or for the period of time necessary to allow a complete verification of the EUT's operating performance.</p> <p>The frequency of the ripple is the power frequency or its multiple 2, 3 or 6, as specified in the product specification.</p> <p>During tests, theDuring the tests, the EUT shall be in operation. Simulated inputs are permitted. Tests shall be performed at a minimum of one flow <u>rateflowrate</u>.</p>	
Percentage of the nominal DC- voltage	2	%
Restrictions	The test level is a peak-to-peak voltage expressed as a percentage of the nominal DC voltage, U_{DC} .	
Permitted maximum deviation	<p>a) Ffor interruptible measuring systems: either significant faults do not occur or checking facilities detect a malfunctioning and act upon in it accordance <u>upon it in accordance</u> with R-117OIML R 117-1, <u>Section 4.3</u> when significant faults occur.</p> <p>b) b) for non-interruptible measuring systems: no significant faults occur.</p>	

Table 4.9.10 Surges on AC and DC mains power lines

Applicable standard	IEC 61000-4-5 [24]			
Test method	Introducing electrical surges on the mains power lines			
Applicability	Only applicable for electronic measuring instruments which are temporarily or permanently connected to a mains power network while in operation			
Object of the test	Verification of compliance with the provisions in R-117 OIML R 117-1, Section 4.1.1 during conditions where electrical surges are superimposed on the mains voltage.			
Test procedure in brief	<p>A surge generator as defined in the referred standard shall be used. The characteristics of the generator shall be verified before connecting the EUT.</p> <p>The test comprises exposure to electrical surges for which the rise time, pulse width, peak values of the output voltage/current on high/low impedance load and the minimum time interval between two successive pulses are defined in the referred standard.</p> <p>At least 3 positive and 3 negative surges shall be applied.</p> <p>On AC mains supply lines the surges shall be synchronised with the AC supply frequency and shall be repeated such that injection of surges on all the 4 phase shifts: - 0°, 90°, 180° and 270° with the mains frequency is covered.</p> <p>The injection network circuit depends on the applicable conductor and is defined in the referred standard.</p> <p>The surges are applied during all the time necessary to perform the test; to that purpose more surges than indicated above may be necessary.</p> <p>During tests, the During the tests, the EUT shall be in operation. Simulated inputs are permitted. Tests shall be performed at a minimum of one flow rate flowrate.</p>			
Test level specifications:	Parameter	mode	value	unit
	Surge voltage peak	Line to line:	1.0	kV
		Line to earth:	2.0	kV
Restrictions	This test does not apply to devices powered by a road vehicle battery.:-			
Permitted maximum deviation	<p>a) Ffor interruptible measuring systems: either significant faults do not occur or checking facilities detect a malfunctioning and act upon in it accordance upon it in accordance with R-117OIML R 117-1, Section 4.3 when significant faults occur.</p> <p>a)b) Ffor non-interruptible measuring systems: no significant faults occur.</p> <p>In either a) or b) above, human intervention is permitted to put the EUT into operation after the test (e.g. replacing a fuse), provided that all relevant data is available after the human intervention.</p>			

Table 4.9.11 Radiated RF electromagnetic fields

Applicable standard	IEC 61000-4-3 [22]; IEC 61000-4-20 [yy]
Test method	Exposure to radiated radio frequency electromagnetic fields
Applicability	Only applicable for electronic measuring instruments containing active electronic circuits
Object of the test	Verification of compliance with the provisions in R-117 OIML R 117-1, Section 4.1.1 under conditions of exposure to electromagnetic fields.
Test procedure in brief	<p>The EUT is exposed to electromagnetic fields with the required field strength and the field uniformity like as defined in the referred standard.</p> <p>The level of field strength specified refers to the field generated by the unmodulated carrier wave.</p> <p>The EUT shall be exposed to the modulated wave field. The frequency sweep shall be made only pausing to adjust the RF signal level or to switch RF-generators, amplifiers and antennas if necessary. Where the frequency range is swept incrementally, the step size shall not exceed 1 % of the preceding frequency value.</p> <p>The dwell time of the amplitude modulated carrier at each frequency shall not be less than the time necessary for the EUT to be exercised and to respond, but shall in no case be less than 0.5 s.</p> <p>Adequate EM fields can be generated in facilities of different type and set-upsetup the use of which is limited by the dimensions of the EUT and the frequency range of the facility.</p> <p>The expected most critical frequencies (e.g. clock frequencies) shall be analyzed separately.</p> <p>During tests, theDuring the tests, the EUT shall be in operation. Simulated inputs are permitted. Tests shall be performed at a minimum of one flowrateflowrate.</p>
Test levels	Test levels may be specified according to R-117 OIML R 117-2 Tables 4.9.11.1 and 4.9.11.2.

Table 4.9.11.1 Electromagnetic fields of general origin

Test level index		2	3	unit
Frequency r Range	(26) 80—1000 MHz	3	10	V/m
Modulation	80 % AM, 1 kHz, sine wave			
Permitted maximum deviation	<p>a) Ffor interruptible measuring systems: either significant faults do not occur or checking facilities detect a malfunctioning and act upon in it accordance <u>upon it in accordance</u> with R-117OIML R 117-1, 4.3 when significant faults occur.</p> <p>b) fFor non-interruptible measuring systems: no significant faults occur.</p>			

Table 4.9.11.2 Electromagnetic fields specifically caused by wireless communication networks

Test level index		3	unit
Frequency r Range	446 MHz ⁽¹⁾	10	V/m
	(0.8—3) GHz ^{(2),(3)}	10	
Modulation	80 % AM, 1 kHz, sine wave		
	<ul style="list-style-type: none">• Applicable only for the Europe region.• The main test level selection criteria should be the consequences of failure of an instrument located at the expected minimum distance from a radiating source for wireless communication. (see sub-clause 8.4.10 and Annex G of IEC 61000-4-3) and the possibility of fraud by using such <u>a</u> radiating source (like such as a mobile phone or a transceiver). Selection of the level indexed 3 is suggested to apply only when the manufacturer of the measuring instrument specifies a minimum distance allowed between licensed communication transmitters and the measuring instrument. In all other cases the level indexed 4 is to be applied.• It is not intended that tests need to be applied continuously over the entire frequency range of (1—6) GHz and may be reduced to cover just the specific frequency bands nationally allocated for RF emitting sources. (see IEC /TR 61000-2-5 [26]. Reduction of the test to cover the frequency range (1.4—3) GHz is expected to cover all wide beam and omni-directional emitting sources.		

Table 4.9.11.3 Conducted (common mode) currents generated by RF EM fields

Applicable standard	IEC 61000-4-6 [25]		
Test method	Injection of RF currents representing exposure to RF electromagnetic fields		
Applicability	Only applicable for electronic measuring instruments containing active electronic circuits and equipped with external electrical wiring (mains power, signal, data and control lines)		
Object of the test	Verification of compliance with the provisions in R-117 OIML R 117-1, <u>Section 4.1.1</u> while exposed to electromagnetic fields.		
Test procedure in brief	<p>An RF EM current, simulating the influence of EM fields shall be coupled or injected into the power ports and I/O ports of the EUT using coupling/decoupling devices as defined in the referred standard.</p> <p>The characteristics of the test equipment consisting of an RF generator, (de-)coupling devices, attenuators, etc. shall be verified before connecting the EUT.</p> <p>During tests, theDuring the tests, the EUT shall be in operation. Simulated inputs are permitted. Tests shall be performed at a minimum of one flow rateflowrate.</p>		
	One of the following test levels may be specified:		
Test level index	2	3	unit
RF amplitude	3	10	V (e.m.f.)
Frequency range	0.15—80		MHz
Modulation	80 % AM, 1 kHz sine wave		
Permitted maximum deviation	<p>a) Ffor interruptible measuring systems: either significant faults do not occur or checking facilities detect a malfunctioning and act upon in it accordanceupon it in accordance with R-117OIML R 117-1, <u>Section 4.3</u> when significant faults occur.;</p> <p>b) fFor non-interruptible measuring systems: no significant faults occur.</p>		

4.54.10 Tests for EUTs powered by a road vehicle battery**Table 4.10.1 Voltage variations**

Applicable standard	ISO 16750-2 [aa]								
Test method	Variation in supply voltage								
Applicability	Applicable to all measuring instruments supplied by the internal battery of a vehicle and charged by use of a combustion engine driven generator								
Object of the test	Verification of compliance with the provisions in R-117 <u>QIML R 117-1, Section 4.1</u> under conditions of high voltage (for example while charging) and low battery voltage.								
Test procedure in brief	The test comprises exposure to the specified maximum and minimum power supply voltage conditions for a period of time necessary for the EUT to be exercised and respond.- The test durations shall be a minimum of one minute.								
	<p>During tests, the During the tests, the EUT shall be in operation. Simulated inputs are permitted. Tests shall be performed at a minimum of one flow-rate <u>flowrate</u>.</p> <p>One of the following test levels may be specified:</p>								
Nominal battery voltage	$U_{nom} = 12\text{ V}$				$U_{nom} = 24\text{ V}$				<u>Units</u>
Test level index	A	B	C	D	E	F	G	H	
Lower limit	6	8	9	10.5	10	16	22	18	V
Upper limit	16	16	16	16	32	32	32	32	V
Notes	<p>1) In ISO 16750-2 [41]- test levels are called “Code”.</p> <p>2) The recommended test level for these tests are: Code C for 12 V batteries and Code F for 24 V batteries.</p>								
Permitted maximum deviation	<p>At both the upper supply voltage level and the lower supply voltage level:</p> <ul style="list-style-type: none"> all functions shall operate as designed. all errors shall be within the maximum permissible errors. 								

Applicable standard	ISO 7637-2 [bb]				
Test method	Electrical transient conduction along supply lines.				
Applicability	Applicable to all measuring instruments <u>which</u> while in operation are supplied by the internal battery of a vehicle which may at the same time be charged by use of a combustion engine driven generator.				
Object of the test	<p>Verification of compliance with the provisions in R-117 <u>QIML R 117-1, Section 4.1.1 under 1</u> under the following conditions (4):</p> <ul style="list-style-type: none"><u>—</u>transients due to a sudden interruption of currents in a device connected in parallel with the device under test due to the inductance of the wiring harness (pulse 2a);<u>—</u>transients from DC motors acting as generators after the ignition is switched off (pulse 2b)(5);transients on the supply lines which occur as a result of the switching processes (pulses 3a and 3b).				
Test procedure in brief	<p>The test comprises exposure to disturbances on the power voltage by direct coupling into the supply lines.</p> <p>During tests, theDuring the tests, the EUT shall be in operation. Simulated inputs are permitted. Tests shall be performed at a minimum of one flow rate<u>flow rate</u>.</p> <p>One of the following test levels may be specified (IV is recommended):</p>				
Test level index	III		IV		Min. number of pulses or test time
Test- pulse	Pulse voltage U_s		Pulse voltage U_s		
	$U_{nom} = 12\text{ V}$	$U_{nom} = 24\text{ V}$	$U_{nom} = 12\text{ V}$	$U_{nom} = 24\text{ V}$	
2a	+37 V	+37 V	+50 V	+ 50 V	500 pulses
2b	+10 V	+20 V	+10 V	+20 V	10 pulses
3a	— 112 V	— 150 V	— 150 V	— 200 V	1 h
3b	+75 V	+150 V	+ 100 V	+ 200 V	1 h
Notes	<p>Test pulse 2b is only applicable when the EUT is connected to the battery via the main switch of the vehicle.</p> <p>So, if the manufacturer of the EUT has not specified that the EUT is connected directly to the battery, test pulse 2b is not applicable.</p> <p>The recommended values in bold, for the level indexed IV, concern the maximum levels as defined in ISO 7637-2 (2004). The values in parentheses are the maximum levels as defined in ISO 7637-2 (2011). (These different test levels are still being debated by the EMC community responsible for ISO 7637-2 for this reason it is recommended to use the the levels outside the</p>				

	parentheses <u>parentheses for the immediate future,</u> Test pulses, minimum of 500 for 2a.
Permitted maximum deviation	<p>a) Ffor interruptible measuring systems: either significant faults do not occur or checking facilities detect a malfunctioning and act upon in it accordance<u>upon it in accordance</u> with R 117<u>OIML R 117-1, Section</u> 4.3 when significant faults occur.</p> <p>b) Ffor non-interruptible measuring systems: no significant faults occur.</p>

Table 4.10.3 Battery voltage variations during starting up a vehicle engine

Applicable standard	ISO 16750-2 [aa]							
Test method	Supply voltage -variation due to energizing the starter motor of a vehicle							
Applicability	Measuring instruments powered by on board DC battery and may be in operation while the vehicle engine is started							
Object of the test	Verification of compliance with the provisions in R 117 <u>OIML R 117-1, Section</u> 4.1. under <u>under</u> conditions of starting the vehicle engine (during and after cranking).							
Test procedure in brief	The test comprises exposure to a typical supply voltage characteristic simulating the voltage variation while cranking the engine using a DC electrical starter motor. During tests, the <u>During the tests, the EUT shall be in operation. Simulated inputs are permitted. Tests shall be performed at a minimum of one flow rate.</u>							
	The following test levels may be specified:							
Nominal battery voltage	$U_{nom} = 12\text{ V}$				$U_{nom} = 24\text{ V}$			Unit
Test profile	I	II	III	IV	I	II	III	
U_S	8	4.5	3	6	10	8	6	V
U_A	9.5	6.5	5	6.5	20	15	10	V
t_8	1	10	1	10	1	10	1	s
t_f	40	100	100	100	40	100	40	ms
Notes	¹⁾ As specified in ISO 16750-2.							
Permitted maximum deviation	<p>a) Ffor interruptible measuring systems: either significant faults do not occur or checking facilities detect a malfunctioning and act upon in it accordance<u>upon it in accordance</u> with R 117<u>OIML R 117-1, Section</u> 4.3 when significant faults occur.</p> <p>b) fFor non-interruptible measuring systems: no significant faults occur.</p>							

Table 4.10.4 “Load dump” test

Applicable standard	ISO 16750-2 [aa]				
Test method	Supply voltage -variation due to disconnecting a discharged battery				
Applicability	Measuring instruments powered by on board DC battery and may be in operation while the vehicle engine is running				
Object of the test	Verification of compliance with the provisions in R-117 <u>ISOIML R 117-1, Section 4.1.4</u> under conditions of disconnecting a discharged vehicle battery while the charging alternator is running.				
Test procedure in brief	The test comprises exposure to a typical pulse on the supply voltage, simulating the voltage peak due to the impedance of connected loads when disconnecting the battery. During tests, the <u>During the tests, the EUT shall be in operation. Simulated inputs are permitted. Tests shall be performed at a minimum of one flow rate</u>				
Nominal battery voltage	$U_{nom} = 12\text{ V}$		$U_{nom} = 24\text{ V}$		unit
Test pulse shape	I	II	I	II	
U_s	80	100	150	200	V
R_i	0.5	4	1	8	V
t_r	10	10	10	10	ms
t_d	40–400	40–400	100–350	100–350	ms
Notes	¹⁾ As specified in ISO 16750-2.				
Permitted maximum deviation	a) f <u>For interruptible measuring systems: either significant faults do not occur or checking facilities detect a malfunctioning and act upon in it accordance upon it in accordance with R-117 <u>ISOIML R 117-1, Section 4.3</u> when significant faults occur.</u> b) F <u>For non-interruptible measuring systems: no significant faults occur.</u>				

5 Testing procedures for meter sensors and measuring devices

5.1 General information

—The meter sensor/measuring device may be tested in either a test bench or in a measuring system. It shall be installed according to the manufacturer's specification (meter position(s), straight pipes, flow straightening device, minimum back pressure, software setting/configuration, warm-up time, etc.). Low-flow cut-off (if applicable) is set at minimum value.

Note: ~~S~~see ~~R-117~~OIML R 117-1, ~~Section~~ 3.1.5.4 on turbine meters and other meter types concerning zero-offset.

Metrological stability shall be achieved before any testing is started. ~~This means that the system shall operate within the repeatability error of Section 3.1.2.2 of R-117~~OIML R 117-1, 3.1.2.2. ~~(S~~see Annex X.5.1 for advice on this~~).~~

—Before conducting tests, it is necessary to evaluate the meter sensor/measuring device by using the general check-list given in ~~R-117~~OIML R 117-3 ~~(to be developed)~~ and the relevant points of the check-list given in Annex ~~X.2.1-X.14~~ (cross reference table to type approval of specific components).

Note: ~~S~~pecific components allowed to receive type approval are only those for which partial MPE²s and/or requirements for acceptance (pass/fail criteria) have been defined.

In accordance with the requirements of ~~Section 6 of R-117~~OIML R 117-1, 6, tests should be carried out at the limits of the rated operating conditions – the limits of pressure, temperature, density, and viscosity. — It is possible to reduce the number of liquids to be tested if it can be shown, through technical analysis of the metering principals, that all requirements are fulfilled for any other liquid.

Definition of meter model:— Different sizes of meter sensors/measuring transducers having family similarities in the principle of operation, construction and materials. — A size is defined by the nominal size of the measuring element of the meter sensor, not the size of the pipe connection.

Meter selection – family of meters

When selecting which sizes of a family of meters are to be tested, the following rules shall be considered:

- ~~T~~he approving authority shall declare the reasons for including and omitting particular meter sizes from testing;
- Mmeters which have the most extreme operating parameters within a family; shall be considered for testing (e.g. the largest flowrate range, the highest peripheral (tip) speed of moving parts, etc.);
- eEndurance tests shall be applied to meters where the highest wear is expected;
- aAll performance tests relating to influence quantities and disturbances shall be carried out on one size from a family of electronic meters;

One way of selecting sizes to test is to use ~~Figure~~ 5.1. — Each line represents one family, meter 1 being the smallest. ~~The family members underlined in Fig-~~ure 5.1 are then selected for testing. — The sizes not tested shall be within the range of $0.5 \times Q_{\max} \leq Q_{\max} \leq 2 \times Q_{\max}$ of the adjacent sizes.




Figure 5.1, Families of Meters Pyramid

Depending on sensor size, the tests to be carried out are as follows (the selection of sizes to be tested shall be justified and explained in the test report):

Table 5.1

Section	Type of test	Selection of meter size to be tested
5.3.1	Reading at zero flowrate	Section 5.3.1 only applies for electro-magnetic, ultrasonic, and massflow meters. - For those meter types, a selection of meter sizes according to Figure 5.1.
5.3.2	Accuracy at metering conditions	A selection of meter sizes according to Figure 5.1.
5.3.3	Accuracy at limits of the working range	If documentary evidence is given that technological similarities exist between sizes, testing is conducted on a reduced number of sizes. See the chart in Annex X, Section X.5.3.3.3 <u>X.5.4.3</u>
5.3.4	Flow disturbance (optional)	Only for meters sensitive to flow profile. This test is not applicable if the verification is performed at its final installation (stated in the type approval certificate). If documentary evidence is given that technological similarities exist between sizes – testing is conducted on a reduced number of sizes.
5.3.5	Inclination test, etc.	Only for drum meters. All sizes.

5.4	Endurance test	<p>Only for meters with moving parts/parts under mechanical stress <u>(this means that Coriolis, ultrasonic, and electromagnetic meters are not required to be tested under Section 5.4).</u></p> <p>Only for those sizes of a model for which the highest wear is expected.</p> <p><i>Note:</i> -The “durability” requirement is met without this endurance test (for meters not actually tested under Section 5.5 because the meter will be running for more than 100 hours during all of the other tests.</p> <p><i>Note:</i> This is a significant change from the endurance requirements of R-117OIML R 117-1. When R-117OIML R 117-2 is approved, R-117OIML R 117-1 will need to reflect this change in a future revision.</p>
5.5	mmq MMQ	A selection of meter sizes according to Figure 5.1 (not applicable for pipeline meters).
5.6	Climate and disturbance tests	One size only in a family.

~~Temporary Convenor Note 1: The project group spent a very significant amount of developing, discussing, editing, and arguing about the “Table showing whether different meter technologies are affected by various operating conditions.” The latest version of this table is found (in lineout form) in Annex X.5.4. The participants at the Teddington meeting (Oct 2013) decided that it was best to not include the table in the 2CD because consensus on its contents could not be reached. The convenor continues to believe that the table would have value if consensus could be reached ... so, it has been left (in lineout form) to encourage Project Group members to comment on whether the table should be included and the table’s suggested practices.~~

5.2 Test equipment

~~—~~To determine the amount of liquid passed through the meter sensor/measuring transducer, a standard test measure (OIML R 120), weighing machine (OIML R 76), pipe prover (OIML R 119) or master meter can be used. Standards, instruments and methods used shall suit the purpose, be traceable to international standards or to national standards traceable to international standards and be part of a reliable calibration program. Any test methods and test volume may be used provided that it is described in the test report and is accompanied by an uncertainty statement/reference to accreditation, demonstrating that the expanded uncertainty is in accordance with ~~Section 4.2~~.

~~—~~The volume of the supply tank shall be of sufficient capacity to not cause foaming of the liquid or a rise in temperature during the tests.

Note: -It is preferable that all gas elimination devices should be vented back to the supply tank to avoid changing the test liquid specifications.

~~—~~The temperature and pressure of the liquid passing through the meter sensor, measuring device or meter shall be measured close to the meter sensor/measuring device.

5.3 Accuracy

5.3.1 Indication at zero flowrate

~~The~~ test for reading at zero flowrate ~~—~~should not exceed ~~line C of OIML R 117-1, Table 2, line C~~ at minimum ~~flow-rate~~flowrate (~~R-117~~OIML R 117-1, ~~Section~~ 3.1.5.4).

Note: ~~Section~~ 5.3.1 only applies for electro-magnetic, ultrasonic, vortex, and massflow meters. ~~For those~~ meter types, apply selection of meter sizes according to ~~Figure~~ 5.1.

5.3.2 Accuracy at metering conditions

5.3.2.1 Accuracy at metering conditions (this section is not applicable to drum meters for alcohol; these meters are covered in 5.3.2.2)

Object of the test

~~—~~The objective of this test is to verify that all individual measurement results at each flowrate meet the requirements concerning the maximum permissible errors.

~~—~~**General information**

~~—~~The ~~flow-rate~~flowrates of the measuring point are defined by:

$$Q = K^{n_F-1} \times Q_{\max}$$

Where n_F is a sequence number of the ~~flow-rate~~flowrate test, and

$$K = \left[\frac{Q_{\min}}{Q_{\max}} \right]^{\frac{1}{N_F-1}}$$

Where N_F is the number of flowrates as in the following table

Q_{\max} / Q_{\min} ratio	N_F
<5	3
5 – 9	5
10 – 12	6
13 – 21	7
22 – 35	8
>35	9

Note 1: ~~For~~ turn-down ratios that are not a whole number, the ratio shall be rounded to the nearest whole number.

Note 2: When testing for an expanded flow range, new test points are added outside the old flow range, without ~~the~~ need to recalculate the old test points.

When $Q_{max}/Q_{min} = 10$, this gives:

$Q(1) = 1.00 \times Q_{max}$	$(0.80 \times Q_{max} < Q(1) < 1.00 \times Q_{max})$
$Q(2) = 0.63 \times Q_{max}$	$(0.56 \times Q_{max} < Q(2) < 0.70 \times Q_{max})$
$Q(3) = 0.40 \times Q_{max}$	$(0.36 \times Q_{max} < Q(3) < 0.44 \times Q_{max})$
$Q(4) = 0.25 \times Q_{max}$	$(0.22 \times Q_{max} < Q(4) < 0.28 \times Q_{max})$
$Q(5) = 0.16 \times Q_{max}$	$(0.14 \times Q_{max} < Q(5) < 0.18 \times Q_{max})$
$Q(6) = 0.10 \times Q_{max}$	$(0.10 \times Q_{max} < Q(6) < 0.11 \times Q_{max})$
$Q(1) = 1.00 \times Q_{max}$	$(0.80 \times Q_{max} \leq Q(1) < 1.00 \times Q_{max})$
$Q(2) = 0.63 \times Q_{max}$	$(0.56 \times Q_{max} < Q(2) < 0.70 \times Q_{max})$
$Q(3) = 0.40 \times Q_{max}$	$(0.36 \times Q_{max} < Q(3) < 0.44 \times Q_{max})$
$Q(4) = 0.25 \times Q_{max}$	$(0.22 \times Q_{max} < Q(4) < 0.28 \times Q_{max})$
$Q(5) = 0.16 \times Q_{max}$	$(0.14 \times Q_{max} < Q(5) < 0.18 \times Q_{max})$
$Q(6) = 0.10 \times Q_{max}$	$(0.10 \times Q_{max} < Q(6) < 0.11 \times Q_{max})$

The above table shows that the set rate of flow through the measurement transducer shall not differ by more than 10% from the calculated ~~flow rate~~flowrate (except at $Q(1)$ where 20% is allowed). Furthermore, the limits for the measurement transducer specified by Q_{max} and Q_{min} shall not be exceeded.

Three independent and identical tests shall be carried out at each ~~flow rate~~flowrate. The result (absolute value) of each of these three tests must not exceed line B of ~~R 117~~R 117-1, Table 2.

The difference between the largest and the smallest results of the three successive measurements (range) is a measure of the repeatability error and shall, according to ~~section OIML R 117-1, 3.1.2.2 and A.6.1 of the International Recommendation R 117-1~~, not be greater than 2/5 of Line A of ~~OIML R 117-1~~, Table 2, for amounts greater than 5 times the minimum measured quantity.

If the measurement transducer is intended to be used together with a mechanical calculator/indicating device:

- tests shall be performed together with that mechanical calculator/indicating device;
- if that mechanical calculator/indicating device has also a price indicating device, the tests shall be performed at two unit prices which correspond to the maximum and minimum torques. This is generally near the maximum and minimum unit prices.
- 1. ~~If the measurement transducer is intended to be used together with a mechanical calculator/indicating device tests shall be performed at two unit prices which correspond to the maximum and minimum torques. This is generally near the maximum and minimum unit prices.~~
- 1. Fill in test report _____ (~~R 117~~R 117-3).
- 2. Draw an error-curve with $-E_{vi}$ as a function of Q for each liquid and each unit price (optional).

5.3.2.2 Accuracy at metering conditions for drum meters for alcohol

For drum meters for alcohol, this test is performed without the sampling device, if applicable.

Meters are tested at the following flow-rates, 3 tests at each flowrate:

Table 4 Drum meter flow rate tests

Drum meter	Flowrate (dm ³ /min)		
	Q_1	Q_2	Q_3
MPE (%)	0,2	0,25	0,3
s Small size (4 L per revolution)	0,5 to 1	1 to 2	2 to 3
B big size (20 L per revolution)	3 to 5	5 to 10	10 to 15

5.3.3 MPE of reserve device (reserve drum) of big size drum meter is 0.6 % at all flowrates.**5.3.3 Accuracy at limits of working range****5.3.3.1 Accuracy at limits of temperature, pressure, viscosity and density**

Perform accuracy tests according to 5.3.2 at limits of temperature, pressure, viscosity and density (when relevant, see ~~R117R-117~~OIML R 117-1, B.A.6.2), limited to 3 flow-rates where, based on review of meter data at metering conditions per 5.3.2, the meter is determined to be least accurate. ~~For electronic meters, these flowrates can be simulated if technically justified.~~

Note: ~~†~~The 3 suggested ~~flow-rate~~flowrates are:

- Q_{\min} ;
- $((Q_{\max} - Q_{\min}) \times 0.25) + Q_{\min}$; and
- Q_{\max} .

State in the ~~pattern-type~~ approval certificate if the meter can be verified in one liquid and used in another ~~etc~~ (~~R117R-117~~OIML R 117-1, 2.6.3).

5.3.3.2 Converted indication within a Coriolis meter

When a Coriolis meter uses its density measurement to calculate the liquid quantity in units of volume or if the density measurement is used by a flow computer as conversion, additional testing is required in addition to 5.3.2.1.

5.3.3.3 When a Coriolis meter uses its density measurement to calculate the liquid quantity in units of volume, next to an indication of mass, the error of the volume indication must also be determined. The accuracy of the converted volume indication is determined at the limits of density according to Section 5.3.2.1 with an MPE of line C of OIML R 117-1, †Table 2, of the ~~R117R-117-1~~ or half of the specified quantity deviation (E_{\min}) in respect to the mass error. In this case, there are no additional requirements to the density.

Note:- As an example, with an accuracy class of 0.3, the MPE on mass is 0.2 and the MPE on volume of a Coriolis meter is 0.1 in respect to the mass error.

~~5.3.3.3 When a coriolis meter uses its density measurement to calculate the liquid quantity in units of volume, next to an indication of mass, the error of the volume indication must also be determined. The accuracy in volume is determined according to 5.3.2.1. with an MPE of line C of table 2 of the ~~R117-1~~ or half of the specified quantity deviation (E_{\min}). In this case there are no additional requirements to the density.~~

~~5.3.3.4~~

~~—— Note: As an example: with an accuracy class of 0.3, the MPE on mass is 0.2 and the MPE on volume is 0.1 in respect to the mass error.~~

5.3.3.4 When in addition to 5.3.3.2.1, the density measurement is used by a flow computer as a conversion, the density accuracy must also be determined in accordance with Section 5.3.3.1.

~~—— When in addition to 5.3.3.2.1, the density measurement is used by a flow computer as conversion, the initial intrinsic error of the density indication must also be determined. This is done at a minimum, medium and maximum density against a reference density with the MPE as stated in table 4.2 of ~~R117-1~~.~~

5.3.4 Flow disturbances ~~-(OIML R 117-1, Sections 3.1.5.2, 3.1.6.1, 3.1.7.1, 3.1.8.1, 3.1.9.1)~~

This test is only to be completed with all the manufacturer's installation requirements followed as described in ~~Section 3.1.5.2 of R-117~~OIML R 117-1, 3.1.5.2.- If appropriate, meters may be tested with at least one flow disturbance, at minimum and maximum flow-rates. Three independent and identical tests shall be carried out at both flow-rates. The E_v of each test must not exceed line A in ~~OIML R 117-1, Table 2 of OIML R-117-1~~OIML R 117-1, without adjustment.

~~Alternative Method~~ **Alternative method 1** ~~Alt-1~~ Use a "half-moon plate" in two orientations, 90° rotated, upstream of the meter. The plate blocks 0.125 ~~x~~* D of the diameter (see OIML R 49-2:2006 and ISO 4064-3:2005).

~~Alternative Method~~ **Alternative method 2** ~~Alt-2~~ Use a ball valve upstream of the meter or the measurement transducer in several valve opening positions (90°, 80°, 65°, 45°).

Other flow disturbance test procedures may also be used, but justification and documentation must be provided. If necessary, additional disturbance configurations may be defined by the technology of the meter.

~~-Note:~~ -See also Annex X.5.3.4.

~~5.3.4.5~~3.5 Drum meters for alcohol

~~5.3.4.15~~3.5.1 Conversion device (~~OIML R 117~~~~R 117~~OIML R 117-1, 3.1.10.3)

—The conversion device of a drum meter for alcohol is tested according to chapter 6, requirements according to OIML R 22, reference temperature 20 °C.

~~5.3.4.25~~3.5.2 Volume of individual measuring chambers (~~OIML R 117~~~~R 117~~OIML R 117-1 3.1.10.1)

—The volume of an individual measuring chamber must not deviate more than $\pm 0.2\%$ from the mean volume.

~~5.3.4.35~~3.5.3 Inclined drum axis (~~OIML R 117~~~~R 117~~OIML R 117-1 3.1.10.1)

—Drum meters for alcohol are tested with drum axis inclined 3° to the horizontal, at minimum ~~flow rate~~~~flowrate~~.

Three independent and identical tests shall be carried out at minimum ~~flow rate~~~~flowrate~~.

—The change in result must not exceed half of line B in ~~OIML R 117-1~~, Table 2 ~~of OIML R 117~~~~R 117-1~~.

~~5.3.4.45~~3.5.4 Test of accuracy of the sampling device (~~OIML R 117-1~~, 3.1.10.4 ~~of R 117~~~~R 117-1~~)

~~Error tests for all sampling ladles are~~Test of error of all sampling ladles is made during one revolution of the drum. MPE of n volumes of ladles (where n is ~~the~~ number of chambers ~~of~~ the drum) is 10 % of the sum of the volumes of all ladles of the drum.

~~5.3.4.55~~3.5.5 Test of volume of the containers (~~OIML R 117~~, 3.1.10.4 ~~of R 117~~~~R 117-1~~)

The error of the volume compared to the nominal volume (stated in the type approval) shall not exceed:

±5 % for the collecting containers (for samples);

—5 % for the volume of the inserting containers (for checking evaporation);

—2.5 % for the surge container (for liquid if the drum ~~gets~~ ~~becomes~~ stuck in the small size meter).

~~5.3.4.65~~3.5.6 Test of accuracy of the thermometer (~~OIML R 117-1~~, 3.1.10.6 ~~of R 117~~~~R 117-1~~)

~~The a~~Accuracy of ~~the~~ thermometer indication maximum temperature (to indicate a too high evaporation ~~rate~~) shall not exceed ± 1 °C.

Note: Tests according to ~~Sections~~ ~~5.34.5.4~~, ~~5.34.5.5~~ and ~~5.34.5.6~~ are not intended for volume measurement; they are intended for revenue.

5.4 Endurance test

—Object of the test

—To determine the long-term stability of the meter sensor/measuring device. This test is only relevant for meters with moving parts.

General information

— An endurance test should be carried out at a flowrate between $0,8 \times Q_{\max}$ and Q_{\max} of the measurement transducer using the liquid the measurement transducer is intended to measure or a liquid with similar characteristics.

— The measurement transducer shall be of the same type and model as used for the accuracy test, but need not be the same individual device. (~~Reference see~~section 5.3.2).

— When the transducer is intended to measure different liquids, the test should be carried out with the liquid that provides the most severe conditions (normally the liquid of lowest viscosity).

— An accuracy test shall precede the endurance test.

— In principle the duration of the endurance test shall be 100 hours in one or several periods. —Details of these test procedures shall be fully documented in the test report (including the choice of test liquid).

— After the endurance test, the measurement transducer is subject to an accuracy test. The deviation between the mean value of the errors after and before the endurance test shall remain within line B of ~~OIML R 117-1~~, Table 2 in ~~OIML R 117-1~~ without any changes of the adjustment or corrections, as specified in ~~section 3.1.2.3 of R 117~~OIML R 117-1, 3.1.2.3.

Test procedure

1. Perform accuracy tests in accordance with 5.3.2 at 3 flowrates (Q_{\min} , $0,25 - 0,40 \times Q_{\max}$, and $0,80 - 1,00 \times Q_{\max}$).
2. Calculate \bar{E}_{vi} (B) for each flowrate.
3. Operate the transducer for 100 hours at a flowrate between $0,8 \times Q_{\max}$ and Q_{\max} . For practical reasons, the volume may be divided up into a number of deliveries.
4. Perform an accuracy test in accordance with 5.3.2 at the same three flowrates. The unit price P_u shall be the same as during the initial accuracy test (only relevant for mechanical calculating/indicating devices).
5. Calculate \bar{E}_{vi} (A) and the difference \bar{E}_{vi} (A) — \bar{E}_{vi} (B) for each flowrate.
6. Fill in test report _____.

Note: If appropriate, the results from the accuracy tests according to 5.3.2 can be used for step 1 of the test procedure. In this situation the middle ~~flow rate~~flowrate is the next lower ~~flow rate~~flowrate from 5.3.2.

5.5 Accuracy on the minimum measured quantity

Object of the test

— To determine the error of volume indication E_{vi} when the transducer delivers the minimum measured quantity.

Note: This testing requirement is not applicable for pipeline applications. — For pipeline meters this test may be replaced by an evaluation/calculation of ~~mmq~~MMQ considering cyclic volume, resolution, time constant and flowrate.

~~General information~~

~~The manufacturer or the applicant for of an OIML cCertificatione offer~~ a measurement transducer ~~has to~~shall define the minimum measured quantity.

~~An accuracy test is made-carried out~~ with a test volume equal to the minimum measured quantity at two flowrates, at Q_{\min} and at the highest attainable flowrate, with standing start and stop (if applicable).

~~Three independent and identical tests shall be carried out at each flowrate.~~

The E_v must not exceed 2 times line B of ~~OIML R 117-1~~, Table 2-~~of OIML R 117~~R 117-1.

Note: The requirements on uncertainty given in ~~section 4.2~~ may not be fulfilled due to a “large” scale interval of indicator of the EUT.

If the measurement transducer is intended to be used together with a mechanical calculator/indicating device:

- tests shall be performed together with that mechanical calculator/indicating device;
- if that mechanical calculator/indicating device also has a price indicating device, the tests shall be performed at two unit prices which correspond to the maximum and minimum torques. This is generally near the maximum and minimum unit prices.

~~If the measurement transducer is intended to be used with a mechanical calculator/indicating device, the tests shall be performed at the unit price which corresponds to the maximum torque. This is generally near the maximum unit price.~~

~~For electronic calculator/indicating devices the set unit price is not relevant.~~

- Fill in test report _____.

5.6 Additional testing procedures for electronic measuring devices (sensor + transducer)

5.6.1 General information

~~For electronic measuring devices, additional tests shall be performed. These tests aim at verifying that the electronic devices comply with the provisions of section 4.1.1 of OIML R 117~~OIML R 117-1, 4.1.1 with regard to influence quantities.

- Performance tests under the effect of influence factors:

When subjected to the effect of influence factors the equipment shall continue to operate correctly and the errors shall not exceed the applicable maximum permissible errors.

- Performance tests under the effect of disturbances:

For interruptible systems, when subjected to external disturbances the equipment shall either continue to operate correctly or detect and indicate the presence of any significant faults. ~~For non-interruptible~~interruptible systems, no significant fault shall occur.

5.6.2 Test equipment

As described in ~~section 5.2~~.

5.6.3 Test procedures

As described in ~~the Section 4~~ with the following remarks:

~~Test only at one flow rate/simulated flow or at “zero flow”, with 3 tests for “Influence” and one test for “Disturbance”.~~

The internal processes in an electronic meter under no-flow conditions are almost identical to those taking place under flowing condition; -therefore, these tests need not be performed under flowing conditions. -Tests under reference conditions should then also be performed under no-flow conditions.

For electromagnetic, Coriolis and ultrasonic flowmeters it is usually necessary to fill the flowsensor with liquid (conductive liquid for electromagnetic flowmeters), ~~liquid~~, to be able to get it in proper operating order.

If the test is performed under no-flow condition, ~~set~~ the low-flow-cut-off and damping shall be set to zero, so changes can be observed.

Temperature measurement:

Electronic meters may be fitted with an internal temperature probe. When the temperature measurement is intended for internal corrections, the device is regarded to be an integral part of the meter, and is included in the testing.

Pressure measurement:

Pressure transmitters may be connected to an electronic meter for various purposes. If intended for correction, the pressure transmitter is considered as a part of the correction device and is included in the testing.

Test under reference conditions

Before the series of tests, the EUT's performance under reference conditions is verified.

For all types of electronic meters, the flowrate indicated under reference conditions is the basis for all further performance tests.

~~5.6.2.1~~

~~5.6.2.25.6.3.1~~ Test ~~m~~Method, ~~i~~nfluence test type A

The object of an influence test is to verify that the electronic meter operates within its maximum permissible errors. Influence tests simulate the instrument's rated operating conditions.

Ambient temperature tests are only relevant when liquid temperature does not "create" the meter temperature completely.

During this type of ~~i~~nfluence test, the meter's flow indication is used to determine if the meter still operates within the MPE's. However, maximum permissible errors apply to volume / mass and not flowrate. By calculating the effect of an observed change in flowrate on the device's minimum flowrate, the maximum influence on a volume / mass measurement is calculated, which must be smaller than the MPE. Expressed mathematically:

$$(\text{change in flowrate} / \text{minimum flowrate}) \times 100\% < \text{MPE}$$

~~Please N~~ote that the effect decreases with increasing flowrate.

~~5.6.2.35.6.3.2~~ Test ~~m~~Method, ~~i~~nfluence test type B

The only difference between an influence test of type A and B is that during a test of type B, the instrument is switched off when the influence factor is applied to the instrument. The instrument's performance is verified after the test. Typically these tests simulate conditions that the instrument is subjected to when it is not operating.

~~5.6.2.45.6.3.3~~ Test ~~m~~Method, ~~D~~isturbance test

The object of a disturbance test is to verify that the instrument's behaviour does not change too much, due to the effects of disturbances. A disturbance test simulates conditions —~~conditions~~ that are not considered to be a rated operating condition.

During the presence of the disturbances, the device's flowrate indication must constantly be monitored for changes. The largest of these changes shall be no larger than the significant fault, when calculated as for ~~i~~influence tests.

EDR

6 Testing ~~p~~Procedures for electronic calculators (that may be equipped with a conversion device), indicating devices, and associated devices

5.76.1 General ~~I~~Information

Tests are performed under reference conditions.

The software and configuration shall be checked according the applicable requirements in ~~Section~~ 4 and the checklist in ~~R-117~~ QIML R 117-3.

Reference tests required in ~~Section~~ 6 are to be conducted before each test and after the final test of the day.

Results of testing conducted in accordance with ~~Section~~ 6 will be recorded in the applicable ~~S~~sections of ~~R-117~~ QIML R 117-3.

6.1.1 Test setup

— For electronic calculators and indication devices, the reference flow can be simulated (for instance by using a motor-driven pulser or electronic pulse simulator). ~~In the case where the indicator is an integrated part of an electronic meter sensor, an electronic offset may be created to simulate a flow indication. Calculators often accept a range of input sensitivity. The calculator input sensitivity must be set to the maximum. Sufficient pulses shall be applied to meet an uncertainty of 1/5 of the MPE fault limit to be verified. It is advisable to apply at least 10_000 pulses to minimize the uncertainty caused by pulse-counting.~~

One of the following approaches shall be used:

First approach:

(When associated measuring devices are included in the evaluation)

Verification of the associated measuring instrument(s) requires that the liquid characteristics are directly applied to the inputs of the associated measuring device(s) (for example a temperature bath for the probe and/or pressure balance for the pressure sensor and/or reference liquid for a densitometer), to provide reference values for temperature, pressure, and density measurements.

Second ~~a~~Approach:

Simulated signals representing temperature, pressure and/or density are applied to the EUT's inputs. The true values for the simulated quantities are derived from the applied reference method (for example, temperature is derived from a resistor in the case of simulated temperature dependent resistances); pressure and or density may be derived from a generated current (in the case of a ~~4—~~20 mA pressure or density input(s)). Density may also be derived from a frequency, in the case of a frequency input.

6.1.2 Accuracy tests

Using an appropriate reference method, the values of the parameter characterizing the liquid are applied to the EUT.

6.1.3 Influence factor tests

For ~~the~~ description of the tests, see ~~Section 4~~:

Dry heat: see 4.8.5

Cold: see 4.8.6

~~Damp heat cyclic: see 4.8.7.~~

Vibration (random): see 4.8.8

AC mains voltage variation: see 4.9.2.1

~~DC mains voltage variation :~~ see 4.9.2.2

~~Voltage variations (road vehicle battery) see 4.10.1~~

During the climate tests, the equipment used for simulation~~g~~ of the deliveries and associated measuring instruments is kept outside the climatic chamber.

For each test the severity levels shall be determined as shown in ~~Chapter 4. A.10.3, A.10.4 and A.11.1 of part 1.~~

~~The test severities for the tests are mentioned in the applicable articles A.10 and A.11 of part 1.~~

~~5.7.16.1.4~~ ~~Electronic d~~Disturbance tests

For the severity levels, see ~~Section 4.9.1.1.~~

For the description of the tests, see the following sections:

~~4.8.7~~ ~~Damp heat, cyclic~~

~~4.9.3:-~~ ~~AC mains voltage dips, short interruptions and voltage variations~~

~~4.9.4:-~~ ~~Bursts (transients) on AC and DC mains~~

~~4.9.5:-~~ ~~Electrostatic discharge (ESD)~~

~~4.9.6:-~~ ~~Fast transients/bursts on signal, data and control lines~~

~~4.9.7:-~~ ~~Surges on signal, data and control lines~~

~~4.9.8:-~~ ~~Voltage dips, short interruptions and voltage variations on DC mains power~~

~~4.9.9:-~~ ~~Ripple on DC input power ports~~

~~4.9.10:-~~ ~~Surges on AC and DC mains lines~~

~~4.9.11.1:-~~ ~~Radiated, radio frequency, electromagnetic fields of general origin~~

~~4.9.11.2:-~~ ~~Radiated, radio frequency, electromagnetic fields specifically caused by digital -telephones~~

4.9.11.3:- Conducted- radio-frequency fields

4.10.2 : ~~_____~~ Voltage variations (road vehicle battery)

4.10.23: Electrical transient conduction along supply lines (road vehicle battery)

In the case of the electromagnetic fields immunity tests, the equipment used for the simulation of the deliveries and associated measuring instruments is kept outside the generated electromagnetic field to prevent the simulation equipment from being disturbed by the RF field.

EDR

5.8.6.2 -Electronic calculators and indicating devices**5.8.16.2.1 Accuracy tests (see tables in ~~R117~~~~R-117~~OIML R 117-3)**

Using an appropriate reference method, three simulated flowrates (frequencies) are applied to the EUT: the minimum, medium and maximum value.

Based on the values applied by means of the reference methods and the volume (or mass, if that is the primary measurement signal) indicated by the calculator / indicating device the indicated value is compared with reference value.

The value of the maximum permissible error for this device is specified in ~~R117~~~~R-117~~OIML R 117-1, ~~Section part 1 clause~~ 2.8.

5.8.26.2.2 -Influence factor testsDry heat test and cold tests

Before, during, and after the dry heat test and cold test, a delivery shall be simulated.

During the dry heat and cold test, the indicated quantity value is compared with the reference value.

Damp heat cyclic test and ~~v~~Vibration test

Before and after the ~~damp heat cyclic test and the~~ vibration test, a simulated delivery is generated.

The indicated quantity value after the ~~damp heat cyclic test and~~ vibration test is compared with the reference value.

During the ~~damp heat cyclic test and the~~ vibration test, the power is switched off.

The value of the maximum permissible error for this device is specified in ~~R117~~~~R-117~~OIML R 117-1, ~~Sectionpart 1 clause~~ 2.8.

~~5.8.3~~**5.8.46.2.3 Electrical ~~d~~Disturbance tests**

Before each test, reference deliveries are generated to determine the intrinsic error.

Damp heat cyclic test

Before and after the damp heat cyclic test, a simulated delivery is generated.

The indicated quantity value after the damp heat cyclic test is compared with the reference value.

During the damp heat cyclic test, the power is switched off.

During the disturbance a simulated delivery is made, and the indication of the indication device is compared with the reference values.

Maximum allowable variation, see ~~R117~~~~R-117~~OIML R 117-1, ~~Section~~ 2.8.

- For interruptible systems: -cChecking facilities shall detect a malfunction and act upon it in accordance with ~~R117~~~~R-117~~OIML R 117-1, ~~Sectionpart 1, clause~~ 4.3.
- For non-interruptible systems: no significant faults shall occur.

5.9.6.3 Conversion device (as part of an electronic calculator)

5.9.16.3.1 First approach

6.3.1.1 Accuracy tests

If regarded as an ~~e~~Electronic ~~C~~conversion ~~D~~device (ECD), the applied associated measuring devices are considered to be an integral part of the conversion device. Consequently, a ~~c~~Conformity ~~A~~assessment is only valid for the EUT, if applied in combination with the associated measuring device submitted with it for ~~C~~conformity ~~A~~assessment.

~~During tests, the~~During the tests, the specific test conditions need to be applied to the ECD including its associated measuring devices, using the reference method.

The indicated converted quantity value is compared with the reference converted value (using an internationally accepted method).

For each of the applicable characteristics of the liquid (i.e. temperature, pressure, density, relative density, etc.) the minimum, medium, and maximum values are applied. Based on the values represented by the simulated signals, the indications of the converted quantities are verified.

Input values used for the verification of the conversion calculation (either the measured unconverted volume or the unconverted volume derived from a simulated input) are assumed to be without error.

~~For the verification of the conversion of the unconverted volume, measured or derived from simulated input, is assumed to be without error.~~

The value of the maximum permissible error for this device is specified in ~~part-OIML R 117-1~~ clause 2.7.1.2.

Note: ~~±The mpe-MPE~~ requirement shall not be less than half of the minimum specified quantity deviation.

~~5.9.1~~6.3.1.2 Influence factor tests

If the transducers and the sensor of the associated measuring devices are separated, only the transducers together with the flowcomputer are placed in the climate room.

For each of the applicable characteristics of the liquid (i.e. temperature, pressure, density, relative density, etc.) the medium value is applied and evaluated.

Dry heat test and cold tests

A delivery is simulated before, during, and after the dry heat test and cold test.

During the dry heat and cold test, the indicated converted quantity value is compared with the reference converted value (using an internationally accepted method).

~~Damp heat cyclic test and~~ Vibration test

A delivery is simulated before and after the ~~damp heat cyclic test and the~~ vibration test.

The indicated converted quantity value after the ~~damp heat cyclic~~ vibration test is compared with the reference converted value (using an international accepted method).

During the ~~damp heat cyclic test and the~~ vibration test, the power is switched off.

The value of the maximum permissible error for this device is specified in ~~part-OIML R 117-1~~ clause 2.7.1.2.

Note: ~~+The mpe-MPE~~ requirement shall not be less than half of the minimum specified quantity deviation.

~~5.9.1.26.3.1.3~~ **Electrical-dDisturbance tests**

Before and during the tests, a simulated delivery is generated.

For each of the applicable characteristics of the liquid (i.e. temperature, pressure, density, relative density, etc.) the medium~~7~~ value is applied and evaluated.

During the tests, the indicated converted value is compared with the reference converted value (using an internationally accepted method).

Before and after each test, a reference non-converted value is generated to determine the intrinsic error.

All of the different components are subject to ~~of~~ the tests.

Damp heat cyclic test

A delivery is simulated before and after the damp heat cyclic test.

The indicated converted quantity value after the damp heat cyclic test is compared with the reference converted value (using an international accepted method).

During the damp heat cyclic test, the power is switched off.

Maximum allowable variation

- For interruptible systems: ~~-The value of the maximum permissible error for this device is specified in part-OIML R 117-1, 4-clause~~ 2.7.1.3.
- For non-interruptible systems: no significant errors shall occur.

~~5.9.26.3.2~~ **Second ~~a~~Approach**

~~5.9.2.16.3.2.1~~ **Accuracy tests of the calculator/conversion device**

Following this second approach for the testing of a conversion device, it is possible to verify separately the accuracy of the associated measuring devices and to verify that the provisions for the calculator / indication device with conversion device are fulfilled.

The values represented by the simulated signals are to be compared with the values indicated by the flowcomputer.

In the case of conversion devices with configurable input sensitivity (measured unit per input signal unit), the input sensitivity must be set to the maximum.

For each of these quantities~~7~~, the minimum, medium, and maximum values are applied. Based on the values represented by the simulated signals, the indications of the quantities are verified~~7~~ (see ~~part-OIML R 117-1, 4-clause~~ ~~Table 4.1~~).

Based on internationally accepted standards and the values represented by the simulated signals, the correctness of the conversion calculation(s) ~~are-is~~ verified~~7~~ (see ~~R-117~~OIML R 117-1, ~~Section~~~~part 1-clause~~ ~~2.7.2.1.3~~).

For the verification of the calculations, tests need ~~to-shall~~ be performed at three ~~values points~~ distributed over the range of the equation. For equations split into sections, three tests in each section ~~need-shallto~~ be performed.

For the verification of the conversion calculation, the measured volume or the volume derived from a simulated input is assumed to be without error.

If the signals to simulate the associated measuring devices are digital, the MPE and significant fault limit of the indications are restricted to rounding errors- (see ~~R-117~~[R-117](#)[OIML R 117-1](#), ~~Section part 1~~, ~~clause 2.7.2.1.1~~).₂

EDR

~~5.9.2.26.3.2.2~~ **Influence factor tests of the conversion/calculator device**

For each of the applicable characteristics of the liquid (i.e. temperature, pressure, density, relative density, etc.), the medium value is applied and evaluated.

Dry heat test and cold tests

Before and after the dry heat test and cold tests, a simulated delivery is generated.

During the dry heat and cold test, the indicated converted quantity value is compared with the reference converted value (using an internationally accepted method).

~~Damp heat cyclic test and~~ Vibration test

Before and after the ~~damp heat cyclic test and~~ vibration test, a simulated delivery is generated.

The indicated converted quantity value after the ~~damp heat cyclic test and~~ vibration test is compared with the reference converted value (using an internationally accepted method).

During ~~cyclic test, and the~~ vibration test, the power is switched off.

Maximum permissible error: see ~~R-117~~OIML R 117-1, ~~Section part 1, clause~~ 2.7.2.1, ~~†~~Table 4.1.

If the signals to simulate the associated measuring devices are digital, the MPE and significant fault limit of the indications are restricted to rounding errors: (see ~~part OIML R 117-1, clause~~ 2.7.2.1.1).

~~5.9.2.36.3.2.3~~ **~~Electronic~~ Disturbance tests of the conversion/calculating device**

Before each test, a simulated reference delivery is generated to determine the intrinsic error.

For each of the applicable characteristics of the liquid (i.e. temperature, pressure, density, relative density, etc.), the medium, value is applied and evaluated.

The equipment used to simulate the signals shall not be influenced by the tests.

The quantities and the conversion calculation are verified using the values represented by the simulated signals and internationally accepted standards.

Damp heat cyclic test

Before and after the damp heat cyclic test, a simulated delivery is generated.

The indicated converted quantity value after the damp heat cyclic test is compared with the reference converted value (using an international accepted method).

During the damp heat cyclic test, the power is switched off.

Maximum allowable variations: see ~~R-117~~OIML R 117-1, ~~Section part 1, clause~~ 2.7.2.1, ~~†~~Table 4.1.

If the signals to simulate the associated measuring devices are digital, the MPE and the significant fault limit of the indications are restricted to rounded errors: (see ~~part OIML R 117-1, clause~~ 2.7.2.1.1).

1. For interruptible systems: -either no significant fault shall occur or the ~~C~~checking facilities shall detect a malfunction and act upon it accordance with ~~R-117~~OIML R 117-1, ~~Section part 1, clause~~ 4.3.

2. For non-interruptible systems: -no significant faults shall occur.

5.10.6.4 Associated ~~m~~Measuring ~~D~~devices

5.10.16.4.1 Accuracy tests of associated measuring devices

The associated measuring device is subjected to a known temperature, pressure or density ~~—or (when applicable) a combination of these at the limits of operation.~~ During the tests, the specific test conditions ~~need-shall~~to be applied to the associated measuring devices using a reference method₇ (for example: ~~-~~a temperature bath and/or pressure balance and/or reference liquid (true values)). Traceable and documented laboratory reference equipment shall be used. ~~-~~ The values indicated by the calculator/indicating device for each of the characteristic quantities shall be used to determine the error for each of the associated measuring devices.

In the case of conversion devices with configurable input sensitivity (measured unit per input signal unit), the input sensitivity must be set to the maximum.

Three values of each of the parameters characterizing the liquid are applied to the EUT: the minimum, ~~medium~~median, and maximum values₈.

Based on the values applied by means of the reference method(s), the correctness of the values for temperature, pressure and/or density indicated on the ~~e~~Electronic ~~C~~conversion ~~D~~device or other indicating device is verified.

Maximum allowable variations: see ~~R-117~~OIML R 117-1, Section-2.7.2.1, Table 4.1 and Section 2.7.2.2.3, Tables 4.2 and 4.3.

5.10.26.4.2 Influence factor tests on associated measuring devices

Dry heat test and cold tests

Before, during, and after the dry heat test and cold tests, the indicated measured value is compared with the reference value.

~~Damp heat cyclic test and~~ Vibration test

Before and after the ~~damp heat cyclic test and~~ vibration tests, the indicated measured value is compared with the reference value.

During ~~damp heat cyclic test and~~ the vibration test, the power is switched off₉.

For each of the applicable characteristics of the liquid (i.e. temperature, pressure, density, relative density, etc.) the medium₇ value is applied and evaluated.

Maximum permissible error: see ~~part~~OIML R 117-1, ~~†~~Tables 4.1, 4.2₁ and 4.3.

5.10.36.4.3 ~~-Electrical d~~Disturbance tests on associated measuring devices

Before each test₁ the indicated value is compared with the reference value to determine the intrinsic error₁.

The reference equipment shall not be influenced by the tests₁.

The correctness of the ~~quantity~~ quantities indications ~~are-is~~ verified by comparing them with the reference values. For each of the applicable characteristics of the liquid (i.e. temperature, pressure, density, relative density, etc.)₁ the medium₇ value is applied and evaluated.

Damp heat cyclic test

Before and after the damp heat cyclic test, the indicated measured value is compared with the reference value.

During the damp heat cyclic test, the power is switched off.

Maximum permissible error: see ~~R-117~~OIML R 117-1, ~~†~~Tables 4.1, 4.2₁ and 4.3.

6.5 Temperature conversion: Tests on the response time of the measuring system temperature sensor.

See ~~R-117~~OIML R 117-1, ~~Sections part 1, clauses~~ 3.7.7 and 6.1.10 for further discussions on these requirements.

The desired temperature change is applied to the EUT using a suitable reference method. The output from the sensor ~~has-shall~~ be able to respond to 90 % of a temperature step change within 15 seconds or (if larger) within a time corresponding to the time needed to deliver, at Q_{\max} , a quantity of twice the MMQ.

In the case of fuel dispensers, this would result in maximum time constants (Tau) as found in the following table:

Table for Section 6.5				
Q_{\max} [L/min]	40	80	130	200
MMQ [L]	5	10	20	50
Time [s]	15.00	15.00	18.46	30.00
Maximum Tau [s]	6.51	6.51	8.02	13.03

~~67~~ **Chapter**—Testing procedures for gas elimination devices

~~6.17.1~~ **1**—General ~~i~~Information

Section 7 covers testing procedures for all three kinds of gas elimination devices mentioned in ~~R 117~~ OIML R 117-1, 2.10: gas separators, gas extractors, special gas extractors.

The gas elimination device may either be type approved as a unit separate from the measuring system (MS) for which it is intended (see 7.2.1), or tested as a unit forming part of MS during type approval of the MS (see 7.2.2).

Note 1:—

In practice, the MS subject to approval or verification is not tested in order to check the performance on gas elimination. In fact, the performance of the gas elimination device is established *a priori* on a specimen of the gas elimination device as a unit separate from the MS for which it is intended. The decision ~~of to~~ fitting a MS with a given kind of gas elimination device is based on an examination considering the worst conditions in which the MS could operate.

Note 2:

For the purpose of ~~this~~ section 7, the term “gas” is used as a general term for “air/gas” or for “mixtures of air and gas”.

Note 3:—

For testing a gas elimination device, usually air is used as the gas introduced into the liquid, but any other appropriate gas (e.g. nitrogen) may be used as well.

In the case that the gas elimination device is a separate unit (see 7.2.1), it is examined whether a type of a gas elimination device complies with the requirements in ~~R 117~~ OIML R 117-1, 2.10.

A specimen of that type must be installed on a suitable test bench. The test bench comprises—, among others, ~~—of~~ a pump upstream of the gas elimination device under test, ~~of~~ a liquid meter and ~~of~~ a standard, both located downstream of the gas elimination device.

The standard of the test bench serves the purpose to determine the volume V_n (without gas) of the delivered liquid without gas; so a suitable standard (e.g. a standard capacity tank) must be used from which gas entrapped in the liquid can escape freely.

The liquid meter of the test bench serves the purpose to determine the volume of both the delivered liquid and of the gas left over in the liquid downstream of the gas elimination device; so the liquid meter is a measure for the efficiency of the gas elimination device, with its meter errors E_{vi} (with gas).

Note: Concerning the type of the liquid meter, positive displacement meters are preferred because of their ability to measure the actual volume of liquid and of gas.

Prior to or after the determination of the meter errors E_{vi} (with gas), the liquid meter ~~has-shall to~~ be tested without gas in order to determine its meter errors E_{vi} (without gas). The difference of the meter errors E_{vi} (with gas) $- E_{vi}$ (without gas) represents the effect due to the influence of gas on the measur~~ementing~~ result. For the purpose of section 7 these values are denoted as the effect of the gas elimination device which shall not exceed the values of ~~R 117~~ OIML R 117-1, 2.10.1.

Note: These values of ~~R 117~~ OIML R 117-1, 2.10.1 do not depend on the accuracy class of the measuring system, but on the type of the liquid.

The type approval certificate of the gas elimination device shall clearly define the kind of gas elimination device which has been tested; in the case of gas separators, information shall be given whether the gas separator has been approved also as a gas extractor.

Note:

According to ~~R 117~~ ISO/IEC 117-1, 2.10.2, a gas separator shall also be approved as a gas extractor if gaseous formations such as gas/air pockets liable to have a specific effect greater than 1 % of the minimum measured quantity can occur as well. So, if such tests have been carried out on the gas separator, the relevant information shall be given in the type approval certificate.

In the case that the gas elimination device is a unit forming part of a MS (see 7.2.2), it shall be examined whether the type of the gas elimination device resp. the individual gas elimination device complies with the requirements in ~~R 117~~ ISO/IEC 117-1, 2.10.

A specimen of that type resp. the individual gas elimination device must be installed in the MS, for which it is intended.

For the standard, the same applies as in the paragraph above.

For the liquid meter, the same applies as in the paragraph above, but the liquid meter is part of the MS; when the liquid meter of the MS is not capable of measuring the actual volume of gas (e.g. meters of the Coriolis type), during the gas elimination device test this liquid meter must be substituted by an appropriate type.

~~6.27.2~~ Testing

7.2.1 Test of a gas elimination device as a separate unit

Tests on gas elimination devices should be carried out for flow-rates up to a maximum of 100 m³/h. For higher ~~flow-rate~~ flowrates, characteristics may be determined by analogy with equipment of the same design and smaller dimensions.

Note:

From long term experience it can be assumed that in general, gas elimination devices for ~~flow-rate~~ flowrates ≤ 100 m³/h comply when their effective volume (volume between inlet and outlet) is ~~as a guide value~~ ≥ 8 % (maybe even less) of the quantity passing through the gas elimination device at Q_{\max} during 1 min.

The test for ~~flow-rate~~ flowrates > 100 m³/h is (~~on for~~ reasons of a lack of appropriate testing facilities for such high ~~flow-rate~~ flowrates) not feasible and therefore it is desirable when the characteristics of big sizes could be determined by analogy to smaller sizes: for gas elimination devices for ~~flow-rate~~ flowrates > 100 m³/h the guide value that they comply with is about twice the above mentioned value of 8 %. ~~N;~~ nevertheless, for the acceptance of the determination by analogy, the manufacturer of the gas elimination device should underpin the assumption of conformity by valuable calculations. ~~T, and the~~ acceptance of these calculations should be up to the authority in charge of type approval.

~~Please Note~~ that for the determination by analogy, parameters ~~like such as the~~ Reynolds number and the Froude number are not acceptable to underpin the assumption of conformity because these parameters are valid only for one-phase-fluids but which are not present when testing gas elimination devices.

The test liquid should either have the viscosity for which the device is intended or a greater ~~one~~ viscosity. If the gas elimination device meets the ~~0,5~~ % criterion in ~~R 117~~ ISO/IEC 117-1, 2.10.1 with a test liquid of a viscosity greater than 1 mPa·s (at 20 °C), no additional tests with a test liquid of a viscosity ≤ 1 mPa·s are required.

As a general rule, the test volume of a test run shall be at least the volume of liquid without gas, delivered during one minute at Q_{\max} of the gas elimination device.

The gas is either introduced by injection downstream of the pump, or by suction upstream of the pump.

- In the case of injection (which makes it possible to operate without changing the performance of the pump due to the entry of gas) the liquid and gas flows are adjusted by means of control valves.
- In the case of suction (which yields a pressure reduction by suction and by this reproduces the conditions in reality) the pump (before gas is added) must be set to Q_{\max} of the gas elimination device

(if the pump flow capacity is higher than needed it has to be adjusted accordingly). The pump should preferably be of the displacement type but it may also be of the centrifugal type if the supply tank feeds the pump by gravity.

The gas flow must then be regulated by a valve positioned upstream of the pump.

~~Temporary Note: — Although “pressure reduction” is in the text of R117R-117-1995, it seems that “gas flow” makes more sense.~~

The gas inlet is fitted with a shut-off/control valve and a non-return valve to prevent liquid from entering the gas inlet and draining out of the of the test bench.

A sight glass is installed in the liquid pipework downstream of the gas inlet and upstream of the gas elimination device in order that the added gas can be observed in the liquid. The added gas has to be clearly visible in the sight glass.

Note:

When testing gas elimination devices, gas and liquid should normally be present as separate phases. ~~T~~; this two-phase-state must be observable (by the sight glass).

If, during the test, the liquid pressure is relatively high (above 2 bar), the gas could ~~get become~~ dissolved in the liquid and this would make the function of removing gas from the liquid in a two-phase-state impossible to test. On the other hand, in order to achieve the required Q_{\max} , it might become necessary to increase the liquid pressure P to a relatively high value (e.g. above 2 bar), with the consequence that the gas ~~becomes gets~~ dissolved (the need for such a (relatively high) pressure may either lie in the characteristic of the test bench or of the gas elimination device or of both).

~~But~~ Even though this testing condition does not correspond to the desired two-phase-state, if the gas elimination device complies at the (relatively high) pressure P and this pressure is defined as the minimum admissible pressure of the gas elimination device, the gas elimination device will also comply when used at any other pressure \geq minimum admissible pressure.

The volume of gas continuously entering the liquid is measured by a gas meter and isothermally converted to atmospheric pressure on the basis of the indication of a manometer fitted upstream of the gas meter.

The liquid pressure must be measured directly downstream of the gas elimination device resp. upstream of the liquid meter to determine the lowest pressure at which the gas elimination device still meets the values in ~~R117R-117~~OIML R 117-1, 2.10.1.

A sight glass, downstream of the gas elimination device, is used to check that the gas is no longer visible in the liquid.

Note: -A slanting in the pipe work downstream of the liquid meter should be avoided to ensure that gas bubbles can escape in the normal way – thus keeping this pipework filled to the same level at the start and at the end of the test.

In the case where the gas elimination device is provided with an automatic stop-valve, the tests ~~have shall to~~ be carried out with this valve installed in the test bench.

Note:

The test report for the gas elimination device has either to indicate the type of this valve or its characteristics concerning the shut off-speed. In the case of pneumatic driven valves, the test report should also indicate the length of the pneumatic control line between the gas elimination device and its automatic stop-valve.

Consequently, the measuring system may either use the indicated type or a type of the same characteristics, and the length of the pneumatic control line shall be \leq -the length indicated by the test report.

~~6.2.1.17.2.1.1~~ Gas separator test

According to ~~R-117~~OIML R 117-1, 2.10.8, a gas separator designed for $Q_{\max} \leq 20 \text{ m}^3/\text{h}$ shall ensure the elimination of any proportion by volume of gases relative to the measured liquid. ~~T~~; the maximum proportion is 30 % gas for gas separators with a ~~Q_{\max}~~ $Q_{\max} > 20 \text{ m}^3/\text{h}$. The volume of gas V_a is measured at atmospheric pressure in determining its percentage.

The gas separator must separate the added gas up to the values in ~~R-117~~OIML R 117-1, 2.10.1, and must stay fully functional.

An example of a test bench which continuously adds gas to the liquid is shown in Advice Annex X.7.4, Figure 1.

Note:

According to ~~R-117~~OIML R 117-1, 2.10.2, a gas separator shall also be approved as a gas extractor in the case where gaseous formations such as gas pockets liable to have a specific effect greater than 1 % of the minimum measured quantity can occur in the measuring system as well. So, if this is the case, the same tests as on gas extractors have to also be performed on gas separators.

~~6.2.1.2~~

~~6.2.1.37.2.1.2~~ Test procedure

All test runs must start and finish with the gas inlet closed and with the delivery pipe of the test bench full and pressurized.

First determine the (relative) errors E_{vi} (without gas) of the liquid meter at least from ~~Q_{\max}~~ Q_{\max} to ~~Q_{\min}~~ Q_{\min} of the gas separator without adding gas, at the minimum pressure achievable on the test bench (e.g. pressure ≤ 2.2 bar) (leading to the error curve of the liquid meter under no gas conditions).

Determine the list of ~~flow-rate~~flowrates according to ~~R-117~~OIML R 117-2, 5.3.2.1.

Then determine the (relative) errors E_{vi} (with gas) of the liquid meter by continuously adding gas to the liquid, in increasing amounts of the gas/liquid ratio up to the maximum proportion (leading to the error curve of the liquid meter under gas conditions). This procedure shall be terminated under the condition of either a) or b):

- a) when it covers the entire range of gas/liquid ratio V_a/V_n ,
- b) when discharge stops automatically.

For each test run at a given gas/liquid ratio start the test run at ~~Q_{\max}~~ Q_{\max} of the gas separator, at the minimum pressure achievable on the test bench, with the gas inlet closed. When ~~Q_{\max}~~ Q_{\max} is reached, introduce gas of the required proportion by regulating the ~~flow-rate~~flowrate of the gas by using the air inlet throttle valve.

Note: The ~~flow-rate~~flowrates of the liquid meter obtained under gas conditions need not be necessarily be the same as under no gas conditions.

Note the gas bubbles in the sight glass of the test bench upstream of the gas separator.

Check the liquid and gas ~~flow-rate~~flowrate together with the pressure values.

- Stop the flow of gas and liquid when the test volume of the liquid is reached; in the case where there is no flow for more than 10 seconds before the test volume of the liquid is reached, close the gas inlet and terminate the test run until the test volume of the liquid is reached.
- Read the liquid volume V_s of the liquid standard and the volume V_i indicated by the liquid meter and calculate V_n . Measurement results gained below ~~Q_{\min}~~ Q_{\min} shall be disregarded.

Convert the (corrected) volume indication $V_{\text{metered gas}}$ of the gas meter at the pressure p_t to the amount of added gas V_a at the atmospheric pressure $p_{\text{atmospheric}}$ by:

$$V_a = \frac{V_{\text{metered gas}} \cdot (p_t + p_{\text{atmospheric}})}{p_{\text{atmospheric}}}$$

In the case of sucked-in gas assume $p_t = 0$.

Calculate the ratio of V_a / V_n and the (relative) meter error $E_{vi}(\text{with gas}) = (V_i - V_n) / V_n$ and determine the difference between $E_{vi}(\text{with gas})$ and $E_{vi}(\text{without gas})$ as the effect of the gas separator due to the added gas.

Note: As the ~~flow-rate~~flowrates of the liquid meter obtained under gas conditions need not ~~be~~ necessarily ~~be~~ the same as under no gas conditions, calculate the difference between the error curve under no gas conditions and the error curve under gas conditions.

~~6.2.1.4~~2.1.3 Gas extractor test

The test bench has a gas reservoir for creating a gas pocket. ~~C;~~ care shall be taken that upstream of the gas extractor the liquid and gas are still present as separate phases and that the injected gas does not ~~get-become~~ dissolved in the liquid (thus conflicting with the test conditions of ~~R-117~~R-117OIML R 117-1, 2.10.9, first paragraph requiring a gas pocket).

The other parts of the liquid pipework upstream of the meter must be kept full. The gas pocket is then added to the liquid at ~~Q_{max}~~Q_{max} of the gas extractor.

The volume of the gas pocket under atmospheric pressure is \geq the minimum measured quantity of the gas extractor.

Note 1: The MMQ of the gas extractor is defined by the applicant, but as a general rule the minimum measured quantity (MMQ) of the gas extractor should be set to a volume corresponding to the flow at Q_{\min} during 1 minute (if only Q_{\max} is known, then Q_{\min} can be derived from the permissible ratio between the maximum and the minimum flowrates of the measuring system according to ~~R-117~~R-117OIML R 117-1, 2.3.3.3).

Note 2:

~~R-117~~R-117OIML R 117-1, 2.10.9, first paragraph requires that the created gas pocket must not be smaller than MMQ, but does not require that the gas pocket is greater than MMQ.

Note 3: The volume of the gas pocket defines the necessary volume of the gas reservoir. ~~I;~~ in the case where the necessary volume at atmospheric pressure $p_{\text{atmospheric}}$ is not provided, the gas pocket may also be created at a pressure p_t , with $p_{\text{atmospheric}} \leq p_t \leq P_{\min}$ of the gas extractor (by then converting the volume of the gas pocket at p_t to the volume of the gas pocket at $p_{\text{atmospheric}}$).

An example of a test bench which adds gas pockets to the liquid is shown in Advice Annex X.7.4, Figure 2.

~~6.2.1.4~~2.1.3.1 Gas pocket test

Make an initial test run without a gas pocket, at ~~Q_{max}~~Q_{max} of the gas extractor and at the minimum pressure.

Note: In order to avoid that gas could get dissolved in the liquid the pressure should be ~~-< 2-2~~ bar.

Then make three test runs by adding the gas pocket of the required volume to the liquid.

Test steps

Vent the liquid pipework completely from entrapped gas and create the gas pocket.

- 1) Perform the test run at ~~Q_{max}~~Q_{max} and the lowest liquid pressure. When ~~Q_{max}~~Q_{max} is reached, open the gas reservoir / the injection valve to discharge the gas pocket into the liquid stream.

- 2) After the gas extractor had acted upon the gas pocket, the ~~flow-rate~~flowrate will resume ~~Q_{\max}~~ Q_{\max} ; continue the delivery at ~~Q_{\max}~~ Q_{\max} and stop it when the test volume of the liquid is reached.
- 3) Read the standard volume V_s and the volume V_i indicated by the meter and calculate V_n from V_s .
- 4) Calculate the meter error E_{vi} (with gas) = $(V_i - V_n)$ and determine the difference between the meter error E_{vi} (with gas) and E_{vi} (without gas) as the absolute error of the gas elimination device due to the added gas.

Note: Gas is not added continuously but only once during the test run, so that E_{vi} (with gas) will occur only once and independently from the delivered liquid volume. Therefore, for the determination of the difference between the meter error E_{vi} (with gas) and E_{vi} (without gas), the absolute (and not the relative) error has to be considered. The difference then must be $\leq 1\%$ of the volume of the added gas pocket.

7.2.1.4 - Special gas extractor test

Note:

Special gas extractors are mainly (but not exclusively) used for measuring systems on road tankers when compartments are completely emptied (operation of the special gas extractor as a gas extractor), but gas can also occur which is continuously and slightly mixed with the liquid (operation of the special gas extractor as a gas separator under the conditions of ~~R-117~~R-117OIML R 117-1, 2.10.9 second paragraph).

For the gas extractor function of special gas extractors not intended for road tankers, the ~~analogue~~analogue tests as on gas extractors described in 7.2.1.2 must be carried out.

For the gas extractor function of special gas extractors intended for road tankers, see 7.2.1.4.

In order to determine the effect of the gas elimination device arising from gaseous formations such as pockets, the supply tank is filled with the test volume. The liquid is then emptied through the meter into the standard without operating the start/stop valve of the test bench. For deliveries not by pump but by gravity, a pipework of the test bench is used which bypasses the pump.

In the case where there is an automatic shut-off valve installed in the liquid pipework of the test bench and operated by the special gas extractor, the gas pocket may be created by emptying the pipework between the supply tank and the gas extractor.

Note: In the case where the test bench has more than one supply tank, a more common way to carry out the gas pocket test is to switch during the delivery to an empty supply tank. ~~T~~the switching test covers the gas pocket test.

For the gas separator function of special gas extractors, the test with continuous gas supply as on gas separators in 7.2.1.1 must be carried out at Q_{\max} of the special gas extractor, but with the gas proportion as defined in ~~R-117~~R-117OIML R 117-1, 2.10.9 second paragraph.

Note:

The maximum achievable ~~flow-rate~~flowrate for MS on road tankers with gravity discharge is normally below ~~Q_{\max}~~ Q_{\max} of the special gas extractor. To reach Q_{\max} of the special gas extractor (in order to meet the requirement of ~~R-117~~R-117OIML R 117-1 for testing at Q_{\max}) the gravity discharge must be supported by simulating an increased static height. This can be accomplished by pressurizing the supply tank. An increase of around 0.4 bar (which could vary due to the ~~used~~test bench ~~used~~) results in a simulated increase of the static height by 4 m). A pressure regulator shall guarantee a stable gas pressure in the supply tank during the tests.

The gas is either injected into the supply pipework or sucked in upstream of the pump, by creating an entry of gas over a gas meter and partly closing the valve of the supply tank.

An example of a test bench which adds to the liquid gas pockets and gas continuously is shown in Advice Annex X.7.4, Figure 3. -This test bench is similar to Figures 1 and 2, but reproduces the actual conditions of deliveries from road tankers to underground tanks, e.g. at petrol stations: the supply tank is located above the special gas extractor and above the meter (i.e. at a level corresponding to that of the road tanker) and the standard is located approximately 4 m below the meter.

~~6.2.1.5~~ 7.2.1.5 Gas extractor function tests of the special gas extractors intended for road tankers (viscosity ≤ 20 mPa.s)

The following tests must be carried out:

- residual discharge test from the supply tank
- gas pocket test
- switching test to an empty supply tank

The switching test to an empty supply tank also covers the gas pocket test.

Notes: The above tests cover all cases where gas pockets on road tankers occur (or might occur) during a delivery:

- ~~The~~ residual discharge test from the supply tank covers the (usual) case where the compartment of a road tanker is completely emptied at the end of a delivery:-
- 7. ~~The~~ gas pocket test covers the case ~~that-where~~ at the start of the delivery gas pockets may occur, e.g. when the pipe between the bottom valve and the special gas extractor is empty, when the measuring system is fed by a compartment on a trailer:-
- 8. ~~The~~ switching test to an empty supply tank (which is the most severe test method for the gas extractor function) covers the cases:-
 - o ~~That-where~~ at the start of the delivery gas pockets may occur, e.g. when the pipe between the bottom valve and the special gas extractor is empty, when the measuring system is fed by a compartment on a trailer;
 - o ~~that-where~~ gas pockets occur at measuring systems without automatic interlock of bottom valves and where one switches during the delivery to an empty compartment.

All tests are carried out according to the specification of the special gas extractor with gravity and pumped discharge.

~~8.1.1.1.1~~ 7.2.1.5.1 Residual discharge test from the supply tank

This test consists of completely emptying a supply tank over the special gas extractor.

Before any test runs are carried out the test bench, including the line from the supply tank, must be vented of any entrapped gas.

One initial test run ~~must-shall~~ be carried out by delivering the liquid quantity until the pipe is empty and the delivery stops without adding gas. Then make three residual discharge test runs.

A test run is carried out with a test volume corresponding to ~~Q_{max}~~ Q_{max} of the special gas extractor during 1 minute. The pipe route is enabled depending on the type of test (gravity discharge or pump operation). During the delivery from the supply tank over the special gas extractor, the supply tank shall run completely empty.

Note:

The same consideration of E_{vi} (with gas) as in 7.2.1.2 applies.

When the special gas extractor is provided with its own automatic stop-valve (which ~~then-shall~~ then be installed in the test bench together with the special gas extractor), the test run is finished when the supply tank

has run completely empty and the special gas extractor ~~doesn't no longer~~ opens its automatic stop-valve ~~any longer~~.

Note:

When the standard is a proving tank and the volume of the delivered liquid is below the nominal capacity of the proving tank, it is necessary to fill ~~up~~ the proving tank ~~up~~ to its nominal capacity. To do ~~so~~ this, the supply tank is refilled and a corresponding volume is delivered at ~~Q_{\max}~~ ~~Q_{\max}~~ into the proving tank without gas being added.

~~8.1.1.1.27.2.1.5.2~~ Gas pocket test

This test consists of delivering a gas pocket over the special gas extractor.

Before any test runs are carried out the test bench, including the gas reservoir, must be vented of any entrapped gas. One initial test run ~~must-shall to~~ be carried out without adding a gas pocket. Then make three gas pocket test runs.

Prepare the gas reservoir with the gas pocket. Switch on the pump and set the test bench to ~~Q_{\max}~~ ~~Q_{\max}~~ of the special gas extractor, then switch to the gas reservoir and discharge the gas pocket into the liquid pipework over the special gas extractor. Resume the test at ~~Q_{\max}~~ ~~Q_{\max}~~ of the special gas extractor to have at least one minute test duration.

Note:

The same consideration of E_{vi} (with gas) as in 7.2.1.2 applies.

~~8.1.1.1.37.2.1.5.3~~ Switching test to an empty supply tank

This test consists of filling one out of two supply tanks with the test liquid and switching the full supply tank to the empty supply tank during the delivery.

Before any test runs are carried out the test bench, including the pipes from the supply tanks, must be vented of any entrapped gas. One initial test run ~~must-shall to~~ be carried out without adding any gas. Then make three switching test runs.

The test is carried out with the volume corresponding to ~~Q_{\max}~~ ~~Q_{\max}~~ for 1 minute. The delivery is started from the filled supply tank over the special gas extractor. The valves in the pipes are switched depending on the type of test (gravity discharge or pump operation).

When the ~~flow rate~~ flowrate reaches ~~Q_{\max}~~ ~~Q_{\max}~~ , the empty supply tank is opened and then the full supply tank is closed.

Continuation of delivery:

- ~~s~~Special gas extractor **with** its own automatic stop-valve:

When the flow is interrupted by the automatic stop-valve, the empty supply tank is closed and the full supply tank is opened again until the volume corresponding to ~~Q_{\max}~~ ~~Q_{\max}~~ during ~~+1~~ minute is delivered;:-

- ~~S~~Special gas extractor **without** its own automatic stop valve:

When no flow is detected for 10 s, the empty supply tank is closed and the full supply tank is opened again until the volume corresponding to ~~Q_{\max}~~ ~~Q_{\max}~~ during 1 minute is delivered.

Note:

The same consideration of E_{vi} (with gas) as in 7.2.1.2 applies. —

~~8.1.27.2.2~~ Tests of a gas elimination device forming part of a measuring system (MS) during type approval of the measuring system

When the gas elimination device is tested in a specimen of the type of the MS, consequently all MS designed according to this type must comply with the specimen regarding the hydraulic conditions under which the gas elimination device ~~works functions properly correctly~~. The pipe-work of the test setup has to be documented.

Notes:

In general, a MS complies with the specimen when:

- Q_{\max} of the MS in use is $\leq Q_{\max}$ under test, and the minimal back pressure of the gas elimination device in use is \geq minimal back pressure under test. In general, this pressure condition is met when the pipework diameter upstream of the gas elimination device in use is \geq the corresponding pipework diameter under test and when the pipework diameter downstream of the gas elimination device in use is \leq the corresponding pipework diameter under test;
- moreover, the negative slope of the pipework downstream of the gas elimination device in use is \leq the corresponding slope under test; any means to prevent the generation of gaseous formations such as anti-swirl devices present in the MS under test shall also be present in the MS in use;
- any means to prevent the generation of a suction downstream of the gas elimination device (e.g. a ventilation valve in an empty hose) present in the MS under test is also present in the MS in use.

Tests on gas elimination devices should be carried out for ~~flow rate~~ flow rates up to Q_{\max} of the MS.

The test liquid should be the same as that for which the measuring system is intended. If the gas elimination device meets the 0,5 % -criterion of ~~R 117~~ ISO/IEC 17025:2014, 2.10.1 with a liquid of a viscosity greater than 1 mPa·s (at 20 °C), no additional tests with a test liquid of a viscosity less than 1 mPa·s are required.

The test volume of a test run shall be at least the volume of liquid without gas, delivered during +1 minute at Q_{\max} of the gas elimination device.

~~8.1.2.1~~ 7.2.2.1 Gas separator tests

This test particularly applies to types of separators included in MS which can be mass produced and transported without dismantling, such as fuel dispensers fed by their own supply pumps.

The essential part of the test bench (see Figure 4) is the MS itself (in this case, the fuel dispenser).

In accordance with conditions encountered in actual use, the liquid is drawn up from the supply tank on a lower level than the meter. The gas is drawn in upstream of the gas separator pump unit by suction through a special inlet equipped with a control valve.

The volume of gas continuously entering the liquid is measured by a gas meter and isothermally converted to atmospheric pressure on the basis of the indication of a manometer fitted upstream of the gas meter. However, it is not necessary to use a gas meter if the gas separator is capable of separating and eliminating the gas introduced in any proportion, as provided in ~~R 117~~ ISO/IEC 17025:2014, 2.10.8.

The requirements in ~~R 117~~ ISO/IEC 17025:2014, 2.10.1 and 2.10.8 shall be complied with under test conditions such that Q_{\max} of the MS is reached when no gas enters.

~~8.1.2.1~~ 7.2.2.1.1 Test procedure for gas separators of fuel dispensers

Note: The tests are carried out in accordance with 7.2.1.1.1.

Note: According to ~~R 117~~ ISO/IEC 17025:2014, 2.10.8, a gas separator designed for $Q_{\max} \leq 20 \text{ m}^3/\text{h}$ shall ensure the elimination of any proportion by volume of gases relative to the measured liquid. As Q_{\max} of fuel dispensers is always $\leq 20 \text{ m}^3/\text{h}$, the fuel dispensers must be tested whether their gas separators are capable of separating and eliminating the gas introduced in any proportion and therefore it is not necessary to determine the percentage of the added gas.

All test runs must start with the gas inlet closed, and with the hose full and pressurized. All test runs must finish with the gas inlet closed and the hose pressurized. If it is expected that the hose has a significant influence ~~to-on the~~ measurement uncertainty of the measurement procedure, the hose has to be replaced by a solid pipe-work.

An example of a test bench which continuously adds gas to the liquid is shown in Advice Annex X.7.4, Figure 14.

First determine the errors E_{vi} (without gas) of the fuel dispenser from ~~Q_{max} Q_{max}~~ to ~~Q_{min} Q_{min}~~ without adding gas:

Set the ~~flow-rate~~flowrate by using a control valve between hose and nozzle, or a nozzle trigger.

Determine the list of ~~flow-rate~~flowrates $Q(n)$ according- to ~~R-117~~R-117OIML R 117-2, 5.3.2.1 from the highest ~~flow-rate~~flowrate $Q(1)$ to the lowest ~~flow-rate~~flowrate $Q(6)$ of the fuel dispenser.

Then determine the errors E_{vi} (with gas) of the fuel dispenser at the same ~~flow-rate~~flowrates as above by continuously adding gas:

- ~~f~~For each test run at ~~flow-rate~~flowrate $Q(n)$, start the test run at ~~Q_{max} Q_{max}~~ of the fuel dispenser:-
- ~~T~~Then introduce air at the suction side of the pump and adjust the ~~flow-rate~~flowrate through the fuel dispenser approximately to the subsequent ~~flow-rate~~flowrate $Q(n+1)$, regulating the ~~flow-rate~~flowrate using the air inlet throttle valve:-

~~S~~Stop the flow of gas and liquid when the test volume of the liquid is reached; in the case where there is no flow for more than 10 seconds before the test volume of the liquid is reached, close the gas inlet and terminate the test run until the test volume of the liquid is reached.

Measurement results gained below $Q(6)$ shall be disregarded.

- 2. ~~r~~Read the liquid volume V_s of the liquid standard and the volume V_i indicated by the liquid meter and calculate V_n from V_s . Measurement results gained below Q_{min} shall be disregarded.

Note: A conversion of the (corrected) volume indication $V_{metered\ gas}$ of the gas meter at the pressure p_t to the amount of added gas V_a at the atmospheric pressure $p_{atmospheric}$ is not necessary in the case of sucked-in gas.

- 3. ~~c~~Calculate the (relative) meter error $E_{vi} \text{ (with gas)} = (V_i - V_n)/V_n$ and determine the difference between $E_{vi} \text{ (with gas)}$ and $E_{vi} \text{ (without gas)}$ as the effect of the gas separator due to the added gas.

~~8.1.2.27~~2.2.2 Gas extractor tests

The MS comprising the gas elimination device must be constructed so that tests can be carried out as described below.

The tests are carried out as in 7.2.1.2.1, but instead of creating a gas pocket in a gas reservoir, either the liquid pipework upstream of the gas extractor, if possible or the gas extractor itself is emptied to an extent that it contains the gas pocket of the required volume.

Note:

The admissible Q_{max} of MS equipped with the tested type of a gas elimination device shall be set equal to or below the maximum achieved flowrate.

~~8.1.2.37~~2.2.3 Special gas extractor tests

The MS comprising the gas elimination device must be constructed so that tests can be carried out as described below.

- **Special gas extractors not intended for MS on road tankers:**

Test of the gas extractor function: The test is carried out as in 7.2.1.2.1, but instead of creating a gas pocket in a gas reservoir, the liquid pipework upstream of the special gas extractors shall be emptied to an extent that it contains the required gas pocket. The test runs shall be carried out at the maximum achievable flowrate.

Note:

The Q_{\max} of MS equipped with the tested type of the gas elimination device shall be set \leq the maximum achieved flowrate.

Test of the gas separator function: The test is carried out as in 7.2.1.1.1, but with the gas proportion as defined in ~~R-117~~ QIML R 117-1, 2.10.9 second paragraph.

Gas is drawn in upstream of the special gas extractor (either by injection or by suction) through a special inlet equipped with a control valve, at the maximum achievable flowrate. The volume of gas is measured by a gas meter.

- **Special gas extractors intended for MS on road tankers:**

Note:

The technology of special gas extractors used for measuring systems on road tankers is such that the effective volume of the evaporation chamber (due to restricted space on road tankers) is small. ~~T;~~ the efficiency of the de-gassing process is supported by an automatic stop-valve (installed downstream of the evaporation chamber and controlled by the special gas extractor), which stops the flow as long as gas of an undue quantity is registered at the special gas extractor.

Therefore, the presence of the automatic stop-valve is an indispensable part of these testing procedures, which are designed for special gas extractors equipped with such automatic stop-valves.

This Recommendation is not intended to prevent the development of new technologies, which might accomplish the same objective without such an automatic stop-valve. ~~F;~~ for such cases, new testing procedures may need to be developed to verify that such a (new technology) special gas extractor meets all of the requirements of ~~R-117~~ QIML R 117-1, 2.10.1 and 2.10.9.

The following tests ~~must~~ shall be carried out:

- ~~r~~Residual discharge test for single compartment and multi compartment road tankers; and
- ~~S~~switching test to an empty compartment for multi compartment road tankers.

These tests will give sufficient evidence that the special gas extractor meets the requirements of ~~R-117~~ QIML R 117-1, 2.10.9 second paragraph (gas extractor function and gas separator function).

When the special gas extractor is presented only on a single compartment road tanker (so that the switching test cannot be carried out), the special gas extractor is only valid for the usage on a single compartment road tanker, unless the compartments of a multi compartment road tanker are locked against simultaneous delivery.

- Residual discharge

The test is carried out by analogy to ~~Section 7.2.1.4.1:~~

A compartment is filled with the test quantity (of at least the quantity delivered in 1 minute at the maximum achievable ~~flow-rate~~ flowrate). The test run is finished when the compartment has run completely empty and the special gas extractor does not open its automatic stop-valve any longer.

Each test run shall be carried out at the nominal ~~flow-rate~~ flowrate of the gas elimination device for pumped discharge and if designed, also for gravity discharge. If the nominal ~~flow-rate~~ flowrate is not achievable, the “achievable” ~~flow-rate~~ flowrate ~~must~~ shall be documented as the maximum ~~flow-rate~~ flowrate.

Test steps:

- 1) Using normal operating means, deliver a quantity from the compartment to be used and allow it to drain until the pipe is empty and the delivery stops.
- 2) Close the compartment and fill it with the test quantity.
- 3) Deliver ~~the~~ the quantity, until the delivery stops.
- 4) Read p_t and T_t at 50 % of the test volume.
- 5) Repeat steps 2–4 twice, and calculate the $E_{vi(\text{with gas})} - E_{vi(\text{without gas})}$.

~~Note 1:~~ The measurement of p_t is not necessary in gravity delivery.

For MS with empty hoses the residual discharge test shall be carried out such that the delivery of the road tanker at a petrol station is simulated: either the standard is placed approx. 3 m beneath the level of the empty hose valve or an under-pressure of approx. 0.3 bar is generated in the hose (e.g. by an acceleration pump).

Care shall be taken that the meter remains completely filled with liquid during the test and ~~that~~ the pressure directly behind the meter does not fall below atmospheric pressure.

- Switching test to an empty compartment

The test is carried out by analogy to ~~7.2.1.4.3:~~

The test set-up is carried out using two compartments A and B of the road tanker. Compartment A is filled with the test quantity (of at least the quantity delivered in 1 minute at the maximum achievable ~~flow-rate~~ flowrate) and compartment B is empty. During emptying compartment A at the maximum achievable ~~flow-rate~~ flowrate, compartment B is opened and compartment A is closed immediately. When the flow is interrupted by the automatic stop-valve, the empty compartment B is closed and the full compartment A is opened again until the test quantity is delivered.

Each test run shall be carried out at the nominal ~~flow-rate~~ flowrate of the gas elimination device for pumped discharge and if designed, also for gravity discharge. If the nominal ~~flow-rate~~ flowrate is not achievable the feasible ~~flow-rate~~ flowrate has to be documented as the maximum ~~flow-rate~~ flowrate.

Test steps:

- 1) Deliver a quantity from compartment A at the maximum achievable ~~flow-rate~~ flowrate.
- ~~1)2)~~ 2) Read p_t and T_t .
- 3) Connect the empty compartment B and then immediately disconnect the filled compartment A.
- 4) After interruption of the delivery, disconnect the empty compartment B and re-connect the filled compartment A.
- 5) Repeat steps 1–4 twice, and calculate $E_{vi(\text{with gas})} - E_{vi(\text{without gas})}$.

~~Note:~~ The measurement of p_t is not necessary in gravity delivery.

98 Test ~~p~~Procedures for ~~A~~ncillary ~~D~~evices

9.18.1 General ~~i~~Information

The test procedures detailed in ~~Section~~ 8 shall only apply to the following ancillary devices:

- ~~p~~Printing devices;
- ~~m~~Memory devices – including ~~d~~Data ~~S~~storage ~~D~~evices (DSDs); and
- ~~c~~Conversion devices (not part of an electronic calculator).

Electronic ancillary devices, as defined in this section, ~~other~~ than purely digital devices as defined in 8.1.1, shall be tested for immunity to electrical disturbance(s).

The influence factor tests for ancillary devices shall comply with the intended use of the device (as specified by the manufacturer).

8.1.1 If the ancillary device is a purely digital device which:

- is not required to ensure correct measurement or intended to facilitate the measuring operations, or
- could not in any way affect the measurement, and
- does not include the power supply for the MI, and
- is equipped with the necessary checking facilities (~~R-117~~~~R-117~~OIML R 117-1, 4.3.5 *Checking facilities for ancillary devices*),

then influence factor tests and disturbance tests do not need to be performed on the hardware of the ~~A~~ncillary device.

8.1.2 For electronic ancillary devices powered by batteries, there is a distinction between the tests for instruments powered by:

- ~~(a)~~ ~~d~~Disposable batteries;
- ~~(b)~~ ~~g~~General rechargeable batteries; and
- ~~(c)~~ ~~b~~Batteries of road vehicles.

In the case of disposable and rechargeable batteries of a general nature, there are no applicable standards available.

Devices powered by non-rechargeable batteries or by rechargeable batteries that cannot be (re)charged during the operation of the measuring system, shall comply with the following requirements:

- ~~t~~The device provided with new or fully charged batteries of the specified type shall comply with the applicable metrological requirements;
- ~~A~~As soon as the battery voltage has dropped to a value specified by the manufacturer as the minimum value of voltage ~~where-at which~~ the device complies with metrological requirements, this shall be detected and acted upon by the device in accordance with ~~Section 4.2 of R-117~~~~R-117~~OIML R 117-1, 4.2.

For these devices, no special tests for disturbances associated with the ~~“mains”~~ power are required.

Devices powered by rechargeable auxiliary batteries that are intended be (re)charged during the operation of the measuring instrument shall both:

- ~~(a)~~ — comply with the requirements for devices powered by non-rechargeable batteries or by rechargeable batteries that cannot be (re)charged during the operation of the measuring- system, with the mains power switched off~~;~~ and
- ~~(b)~~ — comply with the requirements for AC mains powered devices with the mains power switched on.

Devices powered by mains power and provided with a back-up battery for data-storage only~~;~~ shall comply with the requirements for AC mains powered devices.

For electronic devices powered by the on-board battery of a road vehicle, a series of special tests for disturbances associated with the power supply are given in [Section 4.10](#).

Notes:

- ~~a~~Ancillary devices that are powered directly, and not provided with power from/by the measuring device, may be tested as “stand-alone” units~~;~~
- ~~a~~Ancillary devices that are provided with power from/by the measuring device shall be tested installed in a measuring system, or equivalent simulator.

~~9.2.8.2~~ **Disturbance and ~~I~~influence factors tests for ancillary devices**

Note: It is envisaged that the devices in this section would be ~~DIGITAL~~-digital and so ~~I~~influence factors tests, with the exception of mains voltage-~~variations~~ (AC or DC), ~~would not be considered necessary.~~

However, where the device is ~~ANALOGUE~~-analogue~~analog~~ then it is considered that this is addressed in ~~section 8.2.2.~~

~~9.2.18.2.1~~ **Disturbance tests applicable to ~~D~~igital ancillary devices not fulfilling the requirements of —8.1.1, and ~~A~~analogueanalog ancillary devices**

For the severity levels see ~~Section 4.9.1.1.~~

For the description of the tests, see the following sections:

4.8.7 Damp heat, cyclic (condensing)

- 4.9.3 AC mains voltage dips, short interruptions and voltage variations
- 4.9.4 Bursts (transients) on AC and DC mains
- 4.9.5 Electrostatic discharge (ESD)
- 4.9.6 Fast transients/bursts on signal, data and control lines
- 4.9.7 Surges on signal, data and control lines
- 4.9.8 Voltage dips, short interruptions and voltage variations on DC mains power
- 4.9.9 Ripple on DC input power ports
- 4.9.10 Surges on AC and DC mains lines
- 4.9.11.1 Radiated, radio frequency, electromagnetic fields of general origin
- 4.9.11.2 Radiated, radio frequency, electromagnetic fields specifically caused by digital- telephones
- 4.9.11.3 Conducted ~~radio-frequency~~ fields
- 4.10.2 Voltage variations (road vehicle battery)
- 4.10.3 Electrical transient conduction along supply lines (road vehicle battery)

~~9.2.28.2.2~~ **Influence factors -tests applicable to ~~D~~igital ancillary devices not fulfilling the requirements of 8.1.1, and ~~A~~analogueanalog ancillary devices.**

For the severity levels see ~~Section~~ 4.9.1.1.

For the description of the tests, see the following sections:

4.9.2.1 AC mains voltage ~~-~~variation

4.9.2.2 DC mains voltage variation

4.8.5 Dry heat (non-condensing)

4.8.6 Cold

~~4.8.7 Damp heat, cyclic (condensing)~~

4.8.8 Random vibration

~~9.3.18.3~~ **Printing devices**

When the printing device is tested separately from the measuring system, or the simulator, the measuring system or simulator shall not be subject to the test conditions. ~~However,~~ this may not be possible where the printing device is an integral device.

~~The EUT may consist solely of a printing device, or of a printing device connected to a measuring system. The EUT may consist solely of a printing device, or of a measuring system connected to a printing device.~~ During the test, the EUT shall be exposed to the specified condition, ~~while the printing device is operating under reference conditions.~~ ~~During tests, the~~ During the tests, the EUT shall be in operation, simulated inputs (where applicable) are permitted.

The requirements in ~~R-117~~ QIML R 117-1, ~~sections:~~ 3.4, 5.2.7, and ~~5.10.3.1.2~~ shall be satisfied, as applicable.

~~9.3.18.3.1~~ **Disturbance and ~~I~~nfluence factors tests for printing devices (devices not fulfilling the requirements of 8.1.1)**

The classification of the instrument for electrical disturbance tests is given in the first table of ~~Section~~ 4.9.

The relation between the class and the applicable severity levels is given in the second table of ~~Section~~ 4.9.

Disturbance tests are as stated in 8.2.1.

Influence factors tests are as stated in 8.2.2.

A measuring system, or simulator, is operated to establish the primary indications, i.e. a quantity indication and, if applicable, a unit price and price to pay. ~~The EUT shall be in operation during test(s), and a printout shall be initiated.~~

The printout of the primary indications provided by the printing device shall be compared with the indication of the measuring system, or simulator, and shall not deviate from (each of) the primary indications on the measuring instrument, or simulator, by more than one scale interval or the greater of the two scale intervals if they differ (~~R-117~~ QIML R 117-1, 5.10.1.3). ~~The identification (e.g. time /date) for the measurement result data shall be printed.~~

Any value shall be printed as a repeated value from the measuring system or simulator (~~R-117~~ QIML R 117-1, 3.4.7).

Note: ~~p~~Printout is “continuous” during “sweep” of the frequencies, and is not required at each frequency.

~~9.3.28.3.2~~ **Tests for pPrinting Ddevices Powered by a road vehicle battery not fulfilling the requirements of 8.1.1**

The tests for devices powered ~~by from~~ a road vehicle battery are described in ~~Section~~ 4.10.

~~9.3.38.3.3~~ **Checking facilities for pPrinting Ddevices**

At least the following shall be checked:

- presence of paper;
- ~~transmission of data; and~~
- ~~the electronic control circuits (except the driving circuits of the printing mechanism itself)~~
- to ensure the checking facility, of type I or P, operates correctly.

The test shall ensure that the checking facility of the printing device is functioning by an action that forces a printing malfunction. This action should be a simulated incorrectness in the generation, transmission (taking into account ~~R-117~~ QIML R 117-2, 4.3.2.1), processing, or indication of measurement data.

Where the action of the checking facility is a warning, this warning shall be given on the ancillary device concerned or on another visible part of the measuring system.

The requirements in ~~R-117~~ QIML R 117-1, 4.3.1.2 shall be satisfied, as applicable.

8.4 Memory dDevice (e.g. Data Storage Device- DSD)

When the memory device is tested separately the measuring system, or the simulator, shall not be subject to the test conditions, however this may not be possible if the memory device is an integral device.

The EUT may consist solely of a memory device, or of a memory device connected to a measuring system. During the test the EUT shall be exposed to the specified condition. ~~while the memory device is operating under normal atmospheric conditions. During tests, the~~ During the tests, the EUT shall be in operation. ~~S;~~ simulated inputs (where applicable) are permitted.

The test shall ensure that the data stored contains all relevant information necessary to reconstruct an earlier measurement, and be protected against unintentional and intentional changes with common software tools.

These procedures will only check that the data is stored correctly and given back correctly.

The relevant data which are used for a transaction must be stored automatically.

Note: This requirement means that the storing function must not depend on the decision of the person operating the system.

The requirements in ~~R-117~~ QIML R 117-1, ~~sections: 3.5; -4.3.5; -5.10.1.3; and 5.10.3.1.2-~~ shall be satisfied as applicable.

~~9.3.48.4.1~~ **Disturbance and influence factors tests for memory devices not fulfilling the requirements of 8.1.1**

The classification of the instrument for electrical disturbance tests is given in the first table of ~~Section~~ 4.9.

The relation between the class and the applicable severity levels is given in the second table of ~~Section~~ 4.9.

Disturbance tests are as stated in 8.2.1.

Influence factors tests are as stated in 8.2.2.

The measuring system, or simulator, is operated to establish the primary indications, i.e. a quantity indication and, if applicable, a unit price and price to pay. - The EUT shall be in operation during the test(s).

It shall be possible to verify that the stored data corresponds to the data provided by the calculator and that restored data accurately corresponds to stored data.

~~9.3.58.4.2~~ Tests for memory/storage devices not fulfilling the requirements of 8.1.1 powered by a road vehicle battery

The tests for devices powered ~~from~~by a road vehicle battery are described in ~~Section~~ 4.10.

~~9.48.5~~ Conversion devices

The EUT may consist solely of a conversion device or of a conversion device connected to a measuring system. During the test the EUT shall be exposed to the specified condition while the conversion device is operating under normal atmospheric conditions. ~~-During tests, the~~During the tests, the EUT shall be in operation. ~~S~~Simulated inputs (where applicable) are permitted.

Test procedures for conversion devices that are a separate part of a complete measuring system are described in 6.3.2.

When the conversion device is tested separately the measuring system, or the simulator, shall not be subject to the test conditions. ~~-However,~~ this may not be possible if the conversion device is an integral device, in which case ~~section~~ 6.3.1 applies.

The requirements in ~~R-117~~R-117OIML R 117-1, ~~sections: 2.7.1; -2.7.2; -2.9.2; -3.1.10.3; -4.3.5; -5.10.1.3; and 5.10.3.1.2-~~ shall be satisfied as applicable.

~~9.4.18.5.1~~ Accuracy tests for digital conversions devices not fulfilling the requirements of 8.1.1, and analogue conversion devices

The accuracy tests for the conversion device as a separate part of a complete measuring ~~s~~System are described in ~~section~~ 6.3.2 "Second approach".

~~9.4.28.5.2~~ Disturbance and ~~i~~influence factors tests for digital conversions devices not fulfilling the requirements of 8.1.1, and ~~analog~~analog conversion devices

The classification of the instrument for electrical disturbance tests is given in the first table of ~~Section~~ 4.9.

The relation between the class and the applicable severity levels is given in the second table of ~~Section~~ 4.9.

The ~~i~~influence factors tests for the ~~F~~First approach are as stated in ~~section~~ 6.3.1.2.

The ~~D~~Disturbance tests for the ~~F~~First approach are as stated in ~~section~~ 6.3.1.3.

The ~~H~~Hnfluence factors tests for the ~~S~~Second approach are as stated in ~~section~~ 6.3.1.2.

The ~~D~~Disturbance tests for the ~~S~~Second approach are as stated in ~~section~~ 6.3.1.3.

The measuring system, or simulator, is operated to establish the primary indications, i.e. a quantity indication and, if applicable, a unit price and price to pay. -The EUT shall be in operation during the test(s).

~~9.4.38.5.3~~ Tests for digital conversions devices not fulfilling the requirements of 8.1.1, and analog conversion devices powered by a road vehicle battery

The tests for devices powered from a road vehicle battery are described in ~~Section~~ 4.10.

Annex A

Testing procedures for fuel dispensers (type evaluation)

Immediately following this Annex is Annex A-LPG, a separate annex that includes test procedures for LPG dispensers (type evaluation).

Test procedures for initial verification for fuel dispensers and LPG dispensers are not yet complete; drafts of these initial verification test procedures are found in Annex X (Advice and Suggested Practices).

~~Temporary *Note*: a decision to not include initial verification test procedures in the Annexes of the 2CD of ~~R-117~~R 117-2 was made at a Project Group meeting in Teddington in October 2013. Instead, these test procedures are planned to be added as part of the “immediate revision” of all three parts next revision cycle of R117R 117.~~

~~A.1 2) If accuracy tests are performed using a weighing system (ie: using density of test liquid and checking temperature), special care shall be taken to establish relevant uncertainty calculations, and take in consideration the weight of vapours expelled from the test container during fills, and uncertainty on such (see also OIML R120 for additional information). To make this annex easier to read, the expression “measuring standard” is used to designate the calibration means put into use to conduct accuracy tests, whatever those means are. It is understood that the measuring standard is “pre-conditioning” properly before any use (ie: any action to wet, prepare in temperature or other, when needed and/or relevant). Refer to relevant OIML publications for uncertainty assessment and calculation.~~

~~A.2~~A.1 General ~~i~~Information

Test procedures in Annex A are applicable for fuel dispensers and can also be used for other liquid dispensers used ~~on~~at petrol station locations (such as: urea (AUS32/DEF) dispensers, dispensers for windscreen washer fluid (isopropanol/water), and lubricant dispensers) and also boat or small aircraft dispensers, when operation of these is done “hose full.”. Also considered as “similar” ~~is~~ any dispenser for foaming liquid that working in a similar way with “hose full” technique.

Note 1: AUS32 or DEF: Diesel ~~e~~Exhaust ~~F~~fluid is urea at 32 % in water, a post-combustion injection liquid used on some engines to reduce NOx in exhaust. This liquid is not a fuel, but is considered as a liquid other than water, and is distributed ~~on~~at petrol stations along with diesel fuel. Refer to ISO22241 for more details.

Special care shall be taken:

- ~~10~~• when handling AUS32. Refer to health and safety documentation;
- ~~when~~ fluid dries or freezes below ~~–11~~ °C (possible crystallization starting at ~~–5~~ °C).

Note 2: If accuracy tests are performed using a weighing system (i.e.: using density of test liquid and checking temperature), special care shall be taken to establish relevant uncertainty calculations, and take in consideration the weight of vapours expelled from the test container during fills, and uncertainty on such (see also OIML R 120 for additional information). ~~To make this a~~Annex easier

to read, the expression “measuring standard” is used to designate the calibration means put into use to conduct accuracy tests, whatever those means are. It is understood that the measuring standard is “pre-conditioned” properly before any use (i.e. any action to wet, prepare in temperature or other, when needed and/or relevant). Refer to relevant OIML publications for uncertainty assessment and calculation.

~~A.3 —, including AUS32/Diesel Exhaust Fluid (DEF) and blend dispensers. General requirements for the type approval of a complete measuring system are given in Section 6.1.10 of R117-1.~~

~~A.4 — Immediately following this Annex is Annex A-LPG: a separate annex for test procedures for LPG dispensers.~~

~~A.5 — The type approval of a dispenser consists of:~~

~~A.6 — (1) Approving the entire system, and~~

~~A.7 — (2) Verifying that the constituent elements (which have not received separate test reports/type approvals), are compatible and satisfy the applicable requirements.~~

~~A.8 — Appropriate testing procedures for the type approval of a dispenser shall be determined after a full review and consideration of the test reports/type approvals already granted for the constituent elements of the measuring system.~~

~~A.9 — When the constituent elements have not been tested separately nor having received separate type approval, all the tests provided in Sections 4, 5, 6, 7 and 8 shall be performed. When the various constituent elements have all been tested or approved separately, it may be possible to forego type approval testing with a full review of previously issued type approval documentation/drawings of the constituent elements. In this case, it may be appropriate to perform an accuracy tests on the complete measuring system due to the possible influence of hose or hydraulic conditions. Before conducting type approval tests, it is necessary to execute a design evaluation of the dispenser by using the general check-list provided in OIML R117-3.~~

~~A.10~~**A.2 Testing procedures for meters**

Testing is completed in accordance with ~~R117~~[R-117](#)[OIML R 117-2](#), ~~Section 5~~ and (if applicable) ~~Section 6~~. These tests include:

~~Accuracy tests (see Section 5.3...)~~

~~Tests on the MMQ (with maximum specified hose length if applicable) (see Section 5.5...)~~

~~Endurance testing (see section 5.4...)~~

Verification of reverse flow prevention

~~For the reverse flow prevention, during meter testing, systems which are designed to account for reverse flow shall be assessed, and test results shall be recorded in the type approval file (description of solution, e.g.: combination of non return valve and/or reverse pulse counting).~~

~~Note: The purpose of clause 2.13.4 of [R117-1](#) is to ensure that reversal flow cannot influence the next transaction when the system is repressurized. This function is often accomplished with a non return valve. Such a system requires a pressure limiting device to avoid hose or piping rupture. Modern solutions could also utilize reverse pulse counting during idle time of the system, so repressurization does not result in errors greater than the minimum specified quantity deviation.~~

Note: See [Section](#) X.A.2 for additional advice and best practices.

~~A.11A.3~~ Testing procedures for electronic devices: calculator, correction, indicating, and associated devices

Testing is completed in accordance with [Section](#) 6.

A.12A.4 Testing procedures for gas elimination

Testing is completed in accordance with ~~R-117~~R-117OIML R 117-2, ~~Section~~ 7.

If the measuring system is not fitted with a gas elimination device, the requirements of ~~R-117~~R-117OIML R 117-1, ~~Sections~~ 2.10 and 5.1.3 shall be fulfilled. All measurements ~~must~~ shall start with the air inlet closed, and the hose full and pressurized. All measurements ~~shall~~ must finish with air inlet closed and hose pressurized. - (See also ~~Section 7.2.2.1.1 of OIML R-117~~Section 7.2.2.1.1 of OIML R 117-2, 7.2.2.1.1).

Note: ~~Typically~~ Typically submerged pump systems are not fitted with a gas elimination device.

A.13A.5 Testing procedures for ancillary devices

Testing is completed in accordance with ~~Section~~ 8.

A.14A.6 Additional testing procedures for complete fuel dispensers

A.14.1A.6.1 -General requirements

- All tests to be performed with maximum hose length, hose uncoiled.
- All tests to be ~~done-performed~~ on a complete dispenser, if not yet covered by any previous evaluation or, where appropriate, by simulation.
- If remote nozzle arrangement is part of the type evaluation request (secondary transfer point, usually used on ~~h~~H~~S~~S~~truck~~truck lines), testing shall confirm that the requirements of ~~OIML R-117~~OIML R 117-1, ~~section~~ 5.1.7 are fulfilled.

A.14.2A.6.2 Testing procedure related to flow interruption – with maximum specified hose length – ~~o~~Only when mechanical calculator is used

A.14.2.1A.6.2.1-Purpose of the test

To determine effect of sudden pressure variations and flow interruptions on the accuracy of dispensers built with mechanical calculators (applicable MPE is ~~R-117~~R-117OIML R 117-1, Table 2, Line A).

A.14.2.2A.6.2.2-Test procedure

The interruption test shall be performed three times at the maximum flowrate of the fuel dispenser. The test volume shall be comprised between 50% and 100% of volume delivered in one minute at Q_{max} . Using the nozzle, the liquid flow is started and stopped abruptly five times during the same measurement. - These stops shall be made at various time intervals. Results are compared to the reference test of the meter over similar volume.

A.14.3A.6.3 Testing procedures related to fuel dispenser hoses**A.14.3.1A.6.3.1 General**

Hoses do not receive separate type approval (except in some countries where testing is left to national authorities); however, all systems shall fulfil the hose-related requirements of ~~R-117~~ QOIML R 117-1, ~~2.15. The hose dilation shall be less than the allowed hidden quantity. Testing advice on a procedure for a test on hose dilation can be found in the advice Annex X (see also 5.1.14, 6.2.2.1, and B.6.1.10 in R-117 1)~~

A.14.3.2A.6.3.2 Testing procedures related to fuel dispenser hoses - ~~D~~ details

This test is to check that dilation of the maximum specified hose length does not exceed requirements of ~~R-117~~ QOIML R 117-1, ~~2.15.~~

~~d~~Disable hiding of increments at beginning of delivery (see ~~R-117~~ QOIML R 117-1, ~~5.1.14).~~

Note: Action needed at calculator of instrument.

If needed (hose reel present), uncoil hose with ~~neither out~~ starting pump nor pressurizing hose.

Note: Can be done by keeping nozzle boot switch ~~from~~ activating.

~~A~~Activate pump (pressurize hose) and read display change over first 10 seconds.

Note: ~~can be done by activating nozzle boot switch~~ Causes the nozzle boot switch to be activated – record result. Display change corresponds to hose dilation. Check against MPE in ~~R-117~~ QOIML R 117-1, ~~Section 2.15,~~ and record result and whether a hose reel is present or not.

~~F~~For vapor recovery hose: In accordance with ~~R-117~~ QOIML R 117-1, ~~Section 2.18.2,~~ any means to prevent/detect such leak above MPE limits shall be described in the type evaluation checklist approval file.

A.14.4A.6.4 Other fuel dispenser functionality to be tested:**A.14.4.1A.6.4.1 Functional test of communication protocols.****A.14.4.1.1A.6.4.1.1 Test correct communication and retrieving of calculator transaction data with a connected console/POS (when applicable and supplied by manufacturer)****A.6.4.1.2 Test dispenser not accepting new transaction if communication link lost during ongoing transaction:**

- a) Connect dispenser to a console/POS.
- b) Make sure ~~the~~ dispenser mode is “manual authorize from console/POS.”
- c) Initiate and start a transaction.
- d) While transaction is ongoing, disconnect link between console and dispenser.
- e) Hang nozzle – record display indication.
- f) Lift nozzle and check that no further transaction is authorized.
- g) Hang nozzle and check that display still indicates same as last transaction (as per record).

~~A.14.4.1.2~~~~A.6.4.1.3~~ **-Functional test of communication protocols do be ~~done-performed~~ with SSD or console, over remote price change (see ~~R-117~~OIML R 117-1,÷ 3.3.2.1)**

- ~~a~~) Authorization for transaction: program console/POS to not free dispenser automatically.
- ~~b~~) Price (if applicable): program product price for dispenser under test.
- ~~c~~) Lift nozzle: nothing shall happen, except price per unit update according to lifted nozzle (see note).
- ~~d~~) Free dispenser at console/POS.
- ~~e~~) Dispenser calculator shall enter autotest/reset sequence to start transaction.
- ~~f~~) Dispenser display shall display “Volume = zero and ~~p~~Price to pay = zero,” while price per unit of volume displays the product price that was previously set.
- ~~g~~) From the console, try to change the price of ~~the~~ product. It shall not affect the display of the dispenser.
- ~~h~~) Flow some volume in a test can.
- ~~i~~) Hang the nozzle.
- ~~j~~) Display shall remain with same price per unit of volume as set prior to the transaction.
- ~~k~~) At console/POS, carry out usual “cash in” steps for the dispenser. Display of dispenser shall either
~~A.15l) n~~Not change and retain last transaction information~~÷~~ or
~~A.16m) z~~Zero volume and price to pay, and display new price per unit of volume.

Note: ~~R-117~~OIML R 117-1, ~~clause~~ 3.3.2.1~~÷~~ A time of at least 5 seconds shall elapse between indicating a new unit price and before the next measurement operation can start, if the unit price is set from ancillary devices.

~~A.16.1.1~~ ~~A.6.4.2~~ **~~Electronic calibration (Check influence of electronic calibration system)~~**

~~A.16.1.2~~

- ~~Adjust the meter as close as possible to zero setting and record accuracy test result.~~
- ~~Change adjustment by 0.5% using the electronic calibration system (and record need to break any physical seal).~~
- ~~Check result versus accuracy test result of a) (expect change of +0.5% +/- 0.1%).~~
- ~~Change adjustment back to normal (by -0.5%) by using electronic calibration system.~~
- ~~Check result versus accuracy test result of a) (expect result back to 0 +/- 0.1%).~~
- ~~If no physical seal was broken (point b), check electronic log for evidence of both adjustment actions done in b) and d).~~
- ~~Record all results.~~

~~A.16.1.3~~ ~~A.6.4.3~~ **~~Q_{min}~~**

~~A.16.1.4~~

~~— Lift the nozzle, and start a simulated transaction to set flow rate to Q_{min} using control valve (note: such control valve could be placed between hose and nozzle).~~

~~— Stop flow and hang nozzle.~~

~~— Lift nozzle, check reset of display.~~

~~— Perform the accuracy test while checking real flow rate during test.~~

~~— Record the result.~~

~~A.16.1.5~~~~A.16.1.6~~ ~~A.6.4.4~~ ~~Q_{max}~~

~~— Lift the nozzle, and start a simulated transaction to set flowrate to Q_{max} using the control valve (note: such control valve could be placed between hose and nozzle).~~

~~— Stop flow and hang the nozzle.~~

~~— Lift nozzle, check reset of display.~~

~~— Perform the accuracy test while checking real flowrate during test.~~

~~— Record the result.~~

~~A.16.1.7~~~~A.6.4.2~~ A.6.4.5 Accuracy at MMQ

- a) Lift ~~the~~ nozzle, check reset of display. Open ~~the~~ control valve at maximum.

Note: -Such control valve could be placed between hose and nozzle.

- b) Perform the accuracy test at highest achievable flowrate

Note: Achievable means with no spillage.

- c) Record the result.

- d) ~~RR~~Repeat this test to achieve a total of three results.

~~A.16.1.8~~~~A.6.4.3~~ A.6.4.6 Temperature conversion (if applicable)**General**

Temperature compensation when applicable (measurement, probe position, see ~~clauses of OIML R-117~~OIML R 117-2, 6.3, and ~~OIML R-117~~OIML R 117-1, 6.1.10, Note 3). -Testing shall be done in accordance with ~~Chapter 6~~.

Note:- See also ~~Annex X~~A.6.4.6, Annex X for advice and best practices.

~~A.16.1.9~~~~A.6.4.4~~ A.6.4.7 Test of the timeout function

Note: ~~Only~~ applies to dispensers with electronic indicators – see ~~R 117~~R 117OIML R 117-1, ~~section~~ 5.1.15.

- a) Lift the nozzle to activate the dispenser.
- b) Do not deliver fuel – wait for timeout.
- c) Check that dispenser switches off and terminates the transaction within a period not greater than 120 seconds.
- d) Hang the nozzle for 5 seconds.
- e) Lift the nozzle to activate the dispenser.
- f) Deliver a quantity of fuel into the receptacle.
- g) Stop the flow and note the time.
- h) Check that the dispenser switches off and terminates the transaction within a period not greater than 120 seconds.
- i) Hang the nozzle.
- j) ~~Record the result of test of c) and h)~~Record the result of tests c) and h).

~~A.16.2~~A.6.5 Additional testing for ~~b~~Blend dispensers testing – see ~~R 117~~R 117OIML R 117-1, 5.9

~~A.16.2.1~~A.6.5.1 Multigrade dispensers~~Blending gasoline/gasoline~~

An evaluation or testing shall ensure that the accuracy shall meet the MPE requirements at minimum and maximum ratio of mix under normal operating conditions.

~~A.16.2.2~~ Check that the dispenser allows for individual accuracy check of each meter that contributes to the blending.

~~A.16.2.3~~A.6.5.2 Gasoline-oil-dispensers~~Blending gasoline/oil or blending gasoline or diesel with additives~~

~~A.16.2.3.1~~A.6.5.2.1 Oil ~~or~~ additive injected upstream of meter

In this case, oil is measured with the volume of gasoline, and the accuracy of the total volume shall meet MPE requirements ~~at all ratios of mix~~. If ~~oil/additive can use~~ more than one blend ratio can be used, the tests shall be ~~done performed~~ at minimum, maximum, and middle ratio of mix.

~~A.16.2.3.2~~ The oil or additive contribution shall be controlled only if ratio accuracy is to be controlled (see OIML ~~R 117~~R 117-1 clause 5.9.3)

Special means shall be provided in the dispenser to route oil to a special sampling point where the oil volume to be injected is collected and volume measured for test purposes~~verification of the blend ratio~~.

The sSampling point shall be capable of being sealed to prevent fraud.

~~A.16.2.3.3~~A.6.5.2.2 Oil ~~or~~ additive injected downstream of meter

In this case, oil is not measured with the volume of gasoline, and old mix/injection shall be disabled to perform the accuracy test. The accuracy of the total volume test shall meet MPE requirements.

Note: The contribution/volume of oil injected can be checked as additional volume dispensed when oil injection is enabled.

~~A.16.2.3.4 Oil or additive contribution shall be controlled only if ratio accuracy is to be controlled (see OIML R117R 117-1 clause 5.9.3).~~

~~A.16.2.3.5~~

~~A.16.2.3.6 A.6.5.2.2.1 Software alternative: Special adjustment menus needed in the calculator—procedure to be provided by manufacturer.~~

- ~~1. — Test 1 — Disengage oil/additive blend for accuracy test purpose (fuel only) and carry out an accuracy test at Q_{max} .~~
- ~~2. — Test 2 — Engage oil/additive blend at maximum ratio for accuracy test purpose with no correction (ie: oil is injected downstream of the meter but the calculator does not compensate for the volume of oil injected). Carry out an accuracy test at the same Q_{max} and with the same volume as Test 1.~~
- ~~3. — Calculate the difference between test 1 and test 2. The difference is the oil/additive contribution and check versus indicated blend (see R117R 117-1 section 5.9.5 if applicable)~~

~~A.16.2.3.7~~

~~A.16.2.3.8 A.6.5.2.2.2 Physical alternative: special accuracy test process to physically disconnect oil injection and measure it separately—procedure to be provided by manufacturer.~~

Special means shall be provided in the dispenser to route oil to a special sampling point where the oil volume to be injected is collected and volume measured for verification of the blend ratio.

The sSampling point shall be capable of being sealed to prevent fraud.

Annex A-LPG

Testing procedures for LPG dispensers (type evaluation)

~~Definitions for the purpose of this Annex (temporary note: these could be moved to the beginning of R117R-117-2 after review):~~

~~Dynamic flow corrected meters: a meter associated with its transducer, where correction factors linked to flow rate are used to adjust measurement dependently (2 or more factors to optimized the accuracy curve of the measuring system over the flow rate range)~~

~~Measuring standard: generic term to designate the adequate tools (and process) in use to check accuracy of instrument/meter (see note 2). Special care shall be taken to properly assess the ratio of the mix of Butane and Propane in use for any test if it can influence accuracy of measuring standards.~~

~~Console: an ancillary device control system, not in the scope of the type certification, capable of setting the unit price to the dispenser and controlling various phases in self-serving mode on petrol stations (releasing a dispenser, cash-in a dispenser, stop a dispenser, changing price of LPG fuel) using the communication protocol with the dispenser calculator~~

~~LPG dispenser: are considered as LPG dispensers in this annex all commonly used fuel or liquid dispensers where liquid has a saturating vapor pressure above atmospheric pressure at ambient temperature (example is DMF). This included equipment on petrol stations and also used to feed boat or small aircraft, when operation of these is done "hose full."~~

A-L.1 General ~~i~~Information

Test procedures in Annex A-L are applicable for LPG fuel dispensers. ~~General requirements for the type approval of a complete measuring system are given in Section 6.1.10 of R117R-117-1.~~

~~The type approval of a LPG dispenser consists of:~~

- ~~(1) Approving the entire system, and~~
- ~~(2) Verifying that the constituent elements (which have not received separate test reports/type approvals), are compatible and satisfy the applicable requirements.~~

~~Appropriate testing procedures for the type approval of an LPG dispenser shall be determined after a full review and consideration of the test reports/type approvals already granted for the constituent elements of the measuring system.~~

~~When the constituent elements have not been tested separately nor having received separate type approval, all the tests provided in Sections 4, 5, 6, 7 and 8 shall be performed. When the various constituent elements have all been tested or approved separately, it may be possible to forego type approval testing with a full review of previously issued type approval documentation/drawings of the constituent elements. In this case, it may be appropriate to perform accuracy tests on the complete measuring system due to the possible influence of hose or hydraulic conditions. Before conducting type approval tests, it is necessary to execute a design evaluation of the LPG dispenser by using the general check list provided in OIML R117R-117-3.~~

Note: -Special care shall be taken when handling LPG fuel as it can cause severe burns by evaporation.

A-L.2 Testing procedures for meters

~~Preamble-Note:~~ ~~†~~Testing of separate calculator prior to meter testing can be required to use such calculator and associated transducer during meter testing. See A.3.

Testing is completed in accordance with ~~Section 5~~ and (if applicable) ~~Section 6~~. These tests include:

A-L.2.1 Accuracy tests

Determine Q_{\min} and Q_{\max} for ~~the~~ associated viscosity/defined fluid to be measured. It is assumed that any mix of ~~B~~butane/~~P~~ropane is similar to LPG even if the usual specification for such fuel is a mix between 30/70_% and 70/30_% of these two constituents.

Put the meter on the test rig as per ~~the~~ manufacturer's specifications, see ~~OIML R 117-2, section 5.1~~~~R-117~~OIML R 117-2, ~~section 5.1~~. The test rig might include a pump, associated piping, feeding tank, control valves, hose and nozzle. None of these parts shall interfere with the performance of the meter under test. If the test rig is provided by the manufacturer, it shall be capable of ensuring that no air or vapor is fed to the meter during testing (no cavitation).

Adjust ~~the~~ meter to ~~the~~ closest ~~zero-setting~~~~zero-setting~~ at ~~the~~ highest applicable ~~flow-rate~~~~flowrate~~ for approval (or at least 80_% of such value as per ~~the~~ requirement of manufacturer).

If more than one adjustment point is needed, refer to the manufacturer's adjustment procedure (i.e. ÷ in case of multipoint adjustment curve for dynamic adjustment).

Secure adjustment setting~~;~~ it shall remain unchanged for A-L.2.1.7, A-L.2.2 and A-L.2.3. ~~Any change to the adjustment settings of the meter before the end of tests related to section A-L.2.3 will invalidate test results related to section A-L.2.1.7, A-L.2.2 and A-L.2.3. Securing the adjustment setting shall be achieved with adequate seals or isolation of the EUT in a room/building until tests related to section A-L.2.3 are finished.~~

Establish the list of flowrates to be tested as per ~~OIML R 117-2, section 5.3.2.1~~~~R-117~~OIML R 117-2, ~~section 5.3.2.1~~.

Carry out the test for each flowrate (see 5.3.2.1) and record the accuracy test results. All results shall be within ~~the~~ applicable MPE.

Repeat g) at the limits of operation as per ~~OIML R 117-2, clause 5.3.3~~~~R-117~~OIML R 117-2, ~~clause 5.3.3~~.

If applicable, repeat g) with different disturbances as per ~~OIML R 117-2, clause 5.3.4~~~~R-117~~OIML R 117-2, ~~clause 5.3.4~~.

A-L.2.2 Tests on the MMQ (with maximum specified hose length if applicable)÷

Confirm adequate hose arrangement for type evaluation – Flush hose for 3 minutes with continuous flow to remove any remaining air bubbles.

Activate the pumping system to pressurize instrument/meter.

Stop the pump – leave idle for 1 minute.

Reset the indication, activate ~~the~~ pump, pressurize ~~the~~ instrument/meter and deliver a quantity equal to MMQ into the measuring standard at the maximum achievable ~~flow-rate~~~~flowrate~~.

Record the accuracy test result. The result shall be within applicable MPE for MMQ as per clause ~~2.5.1 of OIML R 117-1, 2.5.1~~~~R-117~~OIML R 117-1, ~~2.5.1~~.

Repeat steps b) to e) two more times.

A-L.2.3 Endurance testing - see ~~OIML R-117~~OIML R 117-2, ~~section 5.4~~

If more than one fuel (or extended viscosity range required), the endurance test and related accuracy tests shall be conducted with a fluid having a low viscosity / low lubrication capacity in the viscosity range requested by the manufacturer.

A-L.2.4 Check of reverse flow prevention

During meter testing, systems which are designed to cope with reverse flow shall be assessed, and recorded in the type evaluation file (a description of solution shall be recorded, e.g.: combination of non-return valve and/or reverse pulse counting).

The manufacturer shall provide a test method to demonstrate that the design copes with reverse flow. The test shall be conducted and the result recorded.

Note on ~~OIML R-117~~OIML R 117-1, ~~2.13.4~~:

“2.13.4 When reversal of the flow could result in errors greater than the minimum specified quantity deviation, a measuring system (in which the liquid could flow in the opposite direction when the pump is stopped) shall be provided with a non-return valve. If necessary, the system shall also be fitted with a pressure limiting device.”

It is the purpose of this clause in ~~R-117~~OIML R 117-1 to make sure that reversal flow cannot influence the next transaction when the system ~~gets-becomes~~ repressurized – achieving such a function with a non-return valve. But such a system requires a pressure limiting device to avoid the hose or piping ~~to-bursting~~ open in the event ~~ease~~ of heat overpressure on the hose (sun radiation) or hose overrun. A modern solution can also imply reverse pulse counting during idle time of system, so repressurizing does not result in errors greater than the minimum specified quantity deviation.

A-L.3 Testing procedures for electronic devices: calculator, correction, indicating, and associated devices

Testing is completed in accordance with ~~Section 6~~.

A-L.4 Testing procedures for gas elimination

Testing is completed in accordance with ~~OIML R-117~~OIML R 117-2, ~~Section 7~~.

If the measuring system is not fitted with a gas elimination device, the requirements of ~~R-117~~OIML R 117-1, ~~Sections 2.10 and 5.1.3~~ shall be fulfilled. All measurements must start with the hose full and pressurized. All measurements must finish with the hose pressurized. Apply ~~7.2.2.1.1 of OIML R-117~~OIML R 117-2, 7.2.2.1.1.

Requirements on MPE for gas elimination are in ~~OIML R-117~~OIML R 117-1, ~~section 2.10.1~~.

A-L.5 Testing procedures for ancillary devices

Testing is completed in accordance with ~~Section 8~~.

A-L.6 Additional testing procedures for complete LPG dispensers**A-L.6.1 General requirements**

- All tests shall be performed with maximum hose length, hose uncoiled.

- All tests shall be performed on the complete dispenser, if not yet covered by any previous evaluation or, where appropriate, by simulation.
- If the remote nozzle arrangement is part of the type evaluation request (secondary transfer point, usually used on ~~h~~High ~~S~~speed ~~T~~ruck lines but also possible for dual nozzle arrangement dispenser), testing shall confirm that the requirements of ~~OIML R 117~~R 117-1, ~~section~~ 5.5.5 are fulfilled.

A-L.6.2 Testing procedure related to flow interruption – with maximum specified hose length – ~~O~~only when mechanical calculator is used

A-L.6.2.1 Purpose of the test

To determine effect of sudden pressure variations and flow interruptions on the accuracy of LPG dispensers built with mechanical calculators (applicable MPE is ~~R 117~~R 117-1, Table 2, Line A).

A-L.6.2.2 Test procedure

The interruption test shall be performed three times at the maximum flowrate of the LPG dispenser. The test volume shall be comprised between 50% and 100% of volume delivered in one minute at Q_{max} . Using the “dead man push button” or any internal valve arrangement in the EUT, the liquid flow is started and stopped abruptly five times during the same measurement. – These stops shall be made at various time intervals. Results are compared to the reference test of the meter over similar volume.

A-L.6.3 Testing procedures related to LPG dispenser hoses

A-L.6.3.1 General

Hoses do not receive separate type approval (except in some countries where testing is required by national authorities); however, all systems shall fulfil the hose-related requirements of ~~R 117~~R 117-1, ~~2.15.~~ – The hose dilation and vaporization quantity shall be less than the allowed hidden quantity. – Testing advice on a procedure for a test on hose dilation can be found in the advice Annex X.A.6.2 (see also OIML R 117-1, 5.1.14, 6.2.2.1, and B.6.1.10 ~~in R 117-1~~).

A-L.6.3.2 Testing procedures related to LPG ~~-~~dispenser hoses - ~~D~~etails

The purpose of this test is to check that dilation of the maximum specified hose length does not exceed the requirements of ~~R 117~~R 117-1, ~~Section~~ 2.15.

- ~~1.~~ ~~d~~Disable the hiding of increments at the beginning of the delivery (see ~~R 117~~R 117-1, ~~5.1.14~~).

Note: Action needed at calculator of instrument.

- ~~2.~~ If needed (hose reel present), uncoil the hose without either starting the pump ~~nor~~ pressurizing the hose.

Note: This can be done by keeping the nozzle boot switch activated).

- ~~3.~~ Activate the pump (pressurize hose) and read the display change over the first 10 seconds.

Note 1: This can be done by activating the nozzle boot switch) – record the result. The dDisplay change corresponds to the hose dilation. Check against MPE in ~~R 117~~R 117-1, ~~Section~~ 2.15, and record the result and whether or not a hose reel is present. (see warning, below).

Note 2: ~~O~~en LPG dispensers, controlling the flow (and stopping the flow when desired) may require some training and/or some special arrangement (i.e. ~~a~~ a valve between the nozzle and the hose to stop the flow without disconnecting the safety coupling from the measuring standard).

Warning: ~~W~~When pressurizing the hose, special care shall be taken with the nozzle (as it is not connected to a vehicle). Pressure might create leaks and/or a hazardous situation with nozzle/hose movements.

A-L.6.4 Other LPG dispenser functionality to be tested:

A-L.6.4.1 Functional test of communication protocols

A-L.6.4.1.1 Test correct communication and retrieving of calculator transaction data with a connected console/POS (when applicable and supplied by the manufacturer).

A-L.6.4.1.2 Test that the LPG dispenser is not accepting a new transaction if the communication link is lost during the ongoing transaction.

- Connect the dispenser to a console/POS.
- Make sure the dispenser mode is “manual authorize from console/POS.”
- Initiate and start a transaction.
- While the transaction is ongoing, disconnect the link between the console and the dispenser.
- Hang nozzle – record the display indication.
- Lift nozzle and check that no further transaction is authorized.
- Hang ~~the~~ nozzle and check that the display still indicates the same as the last transaction (as per record).

A-L.6.4.1.3 Functional test of communication protocols to be done with SSD or console, over remote price change (see ~~R-117~~OIML R 117-1, ÷ 3.3.2.1)

- Authorization for transaction: program console/POS to not free dispenser automatically.
- Price (if applicable): program product price for dispenser under test.
- Lift nozzle: nothing shall happen, except price per unit update according to lifted nozzle (see note).
- Free dispenser at console/POS.
- Dispenser calculator shall enter autotest/reset sequence to start transaction.
- Dispenser display shall display “Volume = zero and ~~p~~Price to pay = zero,” while price per unit of volume displays the product price that was set priory.
- From the console, try to change the price of the product. It shall not affect display of dispenser.
- Flow some volume into a test can.
- Hang the nozzle.
- The display shall remain with same price per unit of volume as set priory to transaction.
- At console/POS, carry out usual “cash in” steps for the dispenser. ~~The d~~Display of the dispenser shall either:
 - ~~N~~ot change and retain last transaction information, ÷ or
 - ~~Z~~ero volume and price to pay, and display new price per unit of volume.

Note: ~~OIML R-117~~OIML R 117-1, ~~clause~~ 3.3.2.1: A time of at least 5 seconds shall elapse between indicating a new unit price and before the next measurement operation can start, if the unit price is set from ancillary devices.

~~A-L.6.4.2~~ — ~~Electronic calibration (Check influence of electronic calibration system)~~

- ~~• Adjust meter as close as possible to zero setting and record accuracy test result.~~
- ~~• Change the adjustment by 1% using electronic calibration system (and record need to break any physical seal).~~
- ~~• Check result versus accuracy test result of a) (expect change of +1% +/- 0.2%).~~
- ~~• Change adjustment back to normal (by 1%) by using electronic calibration system.~~
- ~~• Check result versus accuracy test result of a) (expect result back to 0 +/- 0.2%).~~
- ~~• if no physical seal was broken (point b), check electronic log for evidence of both adjustment actions done in b) and d).~~
- ~~• Record all results.~~

~~A-L.6.4.3~~ — ~~Q_{min}~~

- ~~• Lift the nozzle, and start a simulated transaction to set flow rate to Q_{min} using the control valve (such control valve shall be placed between hose and nozzle).~~
- ~~• Stop the flow and hang the nozzle.~~
- ~~• Lift the nozzle, check reset of display.~~
- ~~• Do accuracy test while checking real flow rate during test.~~
- ~~• Record the result.~~

~~A-L.6.4.4~~ — ~~Q_{max}~~

- ~~• Lift the nozzle, and start a simulated transaction to set flowrate to Q_{max} using the control valve (such control valve shall be placed between hose and nozzle).~~
- ~~• Stop flow and hang the nozzle.~~

- ~~Lift the nozzle, check the reset of the display.~~
- ~~Do accuracy test while checking real flowrate during test.~~
- ~~Record the result~~

A-L.6.4.2 ~~A-L.6.4.5~~Accuracy at MMQ

- Lift the nozzle, check reset of display. Open the control valve at maximum (such a control valve shall be placed between the hose and the nozzle).
- ~~Do Perform~~ the accuracy test at the highest achievable flowrate.

Note: Achievable means with no spillage and as per measuring standard arrangement capacity.

- Record the result.
- Repeat the test to achieve three results.

A-L.6.4.3 ~~A-L.6.4.6~~Temperature conversion (if applicable)

A-L.6.4.3.1 ~~A-L.6.4.6.1~~General

Temperature compensation when applicable (measurement, probe position, see ~~clauses of OIML R117R-117~~OIML R 117-2, 6.3, and ~~OIML R117R-117~~OIML R 117-1, 6.1.10, note 3) Testing shall be done performed in accordance with Chapter 6.

Note: Special care shall be taken to properly determine the density of any bButane and Ppropane mix as it can influence the conversion

~~A-L.6.4.4 A-L.6.4.6.2 Method 1: use of a measuring standard capable of correcting also for temperature at final reading (as resulting temperature in a readable information with some measuring standards such as proving cans, with probe sensing LPG temperature in the middle of the volume of liquid).~~

~~A-L.6.4.5~~

~~A-L.6.4.6 Definition of MPEC (Maximum permissible error with correction). MPEC is the addition of applicable line A or B of table 2 of OIML R117R-117-1 and line C for the applicable class (example: if EUT is full LPG measuring system under class 1, MPE is 1% (line A) and conversion extra MPE is 0.4% (line C) as per OIML R117R-117-1 clause 2.7.1.2)~~

~~A-L.6.4.7 Use 2 storage tanks of the same LPG fuel, each at a different temperature. Tank 1 shall be cold, tank 2 shall be warm. The temperature difference between tank 1 and tank 2 shall be at least 10°C. The length of connection piping from tanks to EUT shall be minimal.~~

~~A-L.6.4.8 Pre-condition the measuring standard on tank 1. Adjust meter closest to the zero setting.~~

~~A-L.6.4.9 Execute accuracy test on tank 1. Volume of test shall be at least 2xMMQ + volume of piping and no more than 4xMMQ + volume of piping from tank to EUT. Record result. Result shall be within MPEC.~~

~~A-L.6.4.10 Switch EUT to tank 2. Do not flow liquid from tank 2 unless it is for the next accuracy test.~~

~~A-L.6.4.11 Execute accuracy test on tank 2. Volume of test shall be at least 2xMMQ + volume of piping and no more than 4xMMQ + volume of piping from tank to EUT. Record result. Result shall be within MPEC.~~

~~A-L.6.4.12 Switch EUT to tank 1. Do not flow liquid from tank 2 unless it is for the next accuracy test.~~

~~A-L.6.4.13 Execute accuracy test on tank 1. Volume of test shall be at least 2xMMQ + volume of piping and no more than 4xMMQ + volume of piping from tank to EUT. Record result. Result shall be within MPEC.~~

~~A-L.6.4.14 When applicable, check correction table of calculator (or checksum signature when applicable) and record.~~

~~A-L.6.4.15~~

~~A-L.6.4.16 Notes:~~

~~A-L.6.4.17 The purpose of this Method 1 process is to check global response of Temperature conversion, using measurement standards capable of correcting result with final temperature of transferred LPG fuel. As these means might not be easy to deploy for testing, method 2 allows for split verification for type approval purposes.~~

~~A-L.6.4.18 Special safety precautions shall be in use to prevent LPG hazard when heating.~~

~~A-L.6.4.19~~

~~A-L.6.4.20 A-L.6.4.6.3 — Method 2: split EUT verification for type approval~~

~~A-L.6.4.21~~

~~A-L.6.4.22 Note: These tests can be done with a low hazard fuel such as mineral spirit.~~

~~A-L.6.4.23~~

~~A-L.6.4.24 EUT arrangement shall be with a very short hose.~~

~~A-L.6.4.25 Install reference probe (1) at EUT temperature well.~~

~~A-L.6.4.26 Install reference probe (2) at EUT nozzle spout tip.~~

~~A-L.6.4.27 Disengage temperature correction of EUT (note: refer to manufacturer's manual as this might be the way to have maintenance information displayed on EUT dial such as temperature of fuel at EUT conversion probe).~~

~~A-L.6.4.28 Run flow through the EUT at Q_{max} from the storage tank for at least 3 minutes to stabilize fluid temperature and EUT temperature (outgoing flow can be re-circulated back to the storage tank).~~

~~A-L.6.4.29 Check accurate temperature reading by comparing temperature indicated by the EUT (converted signal from its own temperature probe) with reference probe (1) inserted in the temperature well close to instrument meter/transducer. Maximum difference allowed is 1.3°C (equivalent to 0.4% — line C of table 2 of OIML R117R 117-1 for LPG fuel).~~

~~A-L.6.4.30 Warm up the storage tank by 10°C minimum from actual temperature.~~

~~A-L.6.4.31 Read Probe (1) = PT0, and temperature indicated by EUT = PTS.~~

~~A-L.6.4.32 Initiate flow at Q_{max} and start stopwatch simultaneously.~~

~~A-L.6.4.33 After 15s (+/- 1 second), read Probe (1) = PT1, probe (2)=PT2 and temperature indicated by EUT = PTI.~~

~~A-L.6.4.34 Stop flow.~~

~~A-L.6.4.35 If difference between PT2 and PT1 is greater than 1°C , redo test or re-assess test situation.~~

~~A-L.6.4.36 (PTS-PTI) shall be greater than 90% of (PT1-PT0).~~

~~A-L.6.4.37~~

~~A-L.6.4.38 Note: testing of f) and i) can be arranged outside of the EUT by using a reference bath to compare the EUT probe reading and the reference probe reading. Such an arrangement also allows the full range of temperature to be covered.~~

~~A-L.6.4.39~~

~~A-L.6.4.40~~ A-L.6.4.4 ~~A-L.6.4.7~~ Test of timeout function

Note: ~~e~~Only applies to LPG dispensers with electronic indicators – see ~~R-117~~OIML R 117-1, ~~section 5.1.15~~.

- ~~1.~~ Lift nozzle to activate dispenser.
- ~~2.~~ Do not deliver LPG – wait for timeout.
- ~~3.~~ Check that dispenser switches off and terminates transaction within a period not greater than 120 seconds.
- ~~4.~~ Hang nozzle for 5 seconds.
- ~~5.~~ Lift nozzle to activate dispenser.
- ~~6.~~ Deliver a quantity of LPG into the receiving vessel or back to storage tank.
- ~~7.~~ Stop flow and note time.
- ~~8.~~ Check that dispenser switches off and terminates transaction within a period not greater than 120 seconds.
- ~~9.~~ Hang the nozzle.
- ~~10.~~ Record the result of test of c) and h)Record the result of tests c) and h).

~~A-L-6.4.4.1~~A-L-6.4.5 ~~A-L-6.4.8~~LPG remaining liquid in measuring system (~~OIML R-117~~OIML R 117-1, ~~clause 5.5.2~~)

~~A-L-6.4.4.1.1~~A-L-6.4.5.1 ~~A-L-6.4.8.1~~ General

A stream of LPG ~~under-in~~ gaseous form is created inside the dispenser by the air separator and sent back to the storage tank. This stream of gas is used as a saturating pressure reference. ~~Liquid~~ pressure inside the measuring system shall remain above such reference with a safety factor (e.g. 1 bar safety). For testing, the gas pressure reference (PG) shall be read as it is fed to the pressure maintaining device (see ~~OIML R-117~~OIML R 117-1, 5.5.3 second paragraph). Liquid pressure (PL) shall be read at a point downstream of the aftermeasuring system, and upstream of the downstream pressure maintaining device.

~~A-L-6.4.4.1.2~~A-L-6.4.5.2 ~~A-L-6.4.8.2~~ Test

- Lift ~~the~~ nozzle to activate dispenser and connect to tank return line.
- Read pressure of liquid PL0 and gas phases PG0. PL0 shall be greater than PG0 by at least 1 bar.
- Start flow (activate dead man push button if needed).
- Read pressure of liquid PL1 and gas phases PG1. PL1 shall remain greater than PG1 by at least ~~1~~ 1 bar.
- Close return line of gas from air-separator to storage tank. PG shall be increasing.
- When PG reaches PL, flow of liquid in the measuring system shall stop by activation of the pressure maintaining device.
- Re-open the return line of gas from the air-separator to the storage tank. PG shall decrease, and flow shall resume (unless flow stop was too long and initiated the time-out function).

Annex B

Testing procedures for measuring systems on road tankers

The tests in Annex B apply to measuring systems mounted on road tankers or on transportable tanks for the transport and delivery of all liquids of low viscosity (less than or equal to 20 mPa·s) and stored at atmospheric pressure, with the exception of foaming potable liquids.

Note 1: ~~+~~Tankers for potable liquids are covered in ~~R 117~~R 117OIML R 117-2, Annex E, and tankers for liquefied gasses under pressure will be covered in a future annex.

Note 2: In accordance with ~~Section 2.10.4 of R 117~~R 117OIML R 117-1, 2.10.4, higher viscosity liquids may be covered by ~~Annex~~ Annex B, but are not required to have gas elimination devices fitted. ~~In~~ this case, provision ~~must~~ shall be made to prevent the entry of air into the system.

B.1 General ~~i~~nformation

Measuring systems on road tankers consist of several constituent elements ~~which. These constituent elements~~ may or may not be subject to a separate type evaluation. According to ~~6.1.1 of OIML R 117~~R 117OIML R 117-1, 6.1.1, the constituent elements of a measuring system shall comply with the relevant requirements.

The type evaluation of a measuring system on a road tanker involves verifying that the constituent elements of the system, which have not been subject to separate type approvals, satisfy the applicable requirements.

Tests for carrying out the type evaluation of a measuring system on a road tanker shall therefore be determined on the basis of the type evaluations already granted for the constituent elements.

When none of the constituent elements has been subject to separate type evaluation, all the tests provided in ~~sections~~ 4, 5, 6, 7 and 8 shall be performed.

When all of the various constituent elements have ~~all~~ been evaluated separately, it may be possible to complete type evaluation of the complete measuring system through an evaluation of system drawings and a review of ~~the~~ type evaluation tests of the constituent elements.

Before conducting tests, it is necessary to execute the design evaluation of components and pipe work of the measuring system on a road tanker by using the general check-list given in ~~R 117~~R 117OIML R 117-3 and the relevant points for road tanker evaluation.

B.2 Metrological controls and performance tests for type evaluation of the constituent elements

B.2.1 Testing procedures for meter sensors, measuring devices and meters with mechanical indicating devices

Testing is completed in accordance with ~~Section-5~~. -These tests include:-

- ~~a~~Accuracy tests_{5.2};
- ~~t~~Tests on the minimum measured quantity_{5.2};
- ~~E~~ndurance testing_{5.2} and
- ~~e~~Evaluation of the non-return valve configuration and reverse count detection (~~Section~~see 4.7).

B.2.2 Testing procedures for electronic devices: calculator, correction, indicating, and associated devices

Testing is completed in accordance with ~~Section-6~~.

B.2.3 Testing procedures for gas elimination devices

Testing is completed in accordance with ~~Section-7~~.

Note: ~~If~~ the measuring system is not fitted with a gas elimination device, the _____ requirements of ~~Sections 2.10 and 5.2.3 of R-117~~R-117OIML R 117-1, 2.10 and 5.2.3 shall be fulfilled.

B.2.4 Testing procedures for ancillary devices

Testing is completed in accordance with ~~Section-8~~.

B.3 Metrological controls and performance tests of the complete measuring system

B.3.1 Accuracy test of the complete measuring system

Testing is completed in accordance with ~~Section-5~~. -These tests include:-

- ~~a~~Accuracy tests at Q_{\min} and the maximum achievable flowrate, ~~and~~;
- ~~t~~Tests on the minimum measured quantity (with maximum specified hose length)_{5.2};

B.3.2 Complete emptying of the compartment of a road tanker (single compartment trucks only) – See also Chapter 7.

B.3.2.1 Object of the test

To determine the effect of emptying a compartment of a road tanker during delivery on the accuracy of the quantity indication.

B.3.2.2 Test procedure

The test quantity shall be at least the quantity delivered in one minute at the maximum achievable flowrate-, rounded up to the volume of the test measure used.

(Q_{\max} is often impossible to achieve if the system has gravity delivery).

A compartment of a road tanker, filled with the volume of the test measure used, is completely emptied until the delivery stops. The test shall be performed three times at the maximum achievable flowrate of the measuring system.

Using normal operating means, deliver a quantity from the compartment to be used and allow it to drain until the pipe work is empty and delivery stops by itself.

- 1) Wet and drain the test measure (if not correctly done after delivering the product in step 1).

- 2) Close the compartment and fill it with a quantity of product equal to the volume of the test measure.
- 3) Reset the indication of the CID.
- 4) Fill the test measure at Q_{\max} (or at the maximum achievable flowrate of the measuring system) until the delivery is interrupted.
- 5) Read p_t and T_t at 50 % of the test volume.
- 6) Read V_i , V_s , and T_s .
- 7) Calculate V_n and E_{vi} .
- 8) Drain the test measure.
- 9) Repeat steps 3 to 9 twice, and calculate the mean value \bar{E}_v .
- 10) Fill in the test report.

Note: The detection of p_t is not necessary in gravity delivery.

B.3.3 Connecting of an empty compartment (multiple compartment trucks only)

B.3.3.1 Object of the test

To determine the effect of connecting an empty compartment of a road tanker during delivery on the accuracy of the quantity indication.

B.3.3.2 Test procedure

The test shall be performed three times at the maximum achievable flowrate of the measuring system. -The test quantity shall be at least the volume delivered in one minute at the maximum achievable flowrate.

The delivery starts from a filled compartment of the road tanker. After at least one minute, an empty compartment is connected and the filled compartment is disconnected. After the delivery stops, the empty compartment is disconnected, the filled compartment is connected and the delivery is continued until the test measure is filled.

- 1) Wet and drain the test measure.
- 2) Reset the indication of the CID.
- 3) Start the filling procedure of the test measure from the filled compartment at the maximum achievable flowrate.
- 4) Read p_t and T_t .
- 5) Connect the empty compartment and disconnect the filled compartment.
- 6) After interruption of the delivery disconnect the empty compartment, connect the filled compartment and fill the test measure to its nominal volume.
- 7) Read V_i , V_s , T_s .
- 8) Calculate V_n and E_{vi} .
- 9) Drain the test measure.
- 10) Repeat steps 2 to 9 twice, and calculate the mean value \bar{E}_v .
- 11) Fill in the test report

Note: The detection of p_t is not necessary in gravity delivery.

B.3.4 Variation in the internal volume of the hose (full hose measuring systems only)

B.3.4.1 Object of the test

To determine the effect of the increase in internal volume of a hose under pressure on the accuracy of the quantity indication.

B.3.4.2 General information

The manufacturer may provide information on how the requirement in ~~Section 2.15 of~~ OIML ~~R117~~R-117R ~~117-1, 2.15~~ is fulfilled. ~~It may consist in providing the reference of the hose if it has been used previously in an approved measuring system or results of tests performed by the manufacturer of the measuring system or of the hose.~~

It shall then be verified that the hose is not used in worse conditions (pressure, length) than previously tested. If the manufacturer is not able to provide this information, testing is necessary.

— A hose is characterized by:

- a) Manufacturer;
- b) Designation;
- c) Inner diameter;
- d) Length of the hose;
- e) The test report shall further contain data concerning:
 - Maximum operating pressure of the measuring system; and
 - Minimum measured quantity of the measuring system.

B.3.4.3 Test equipment:

Calibrated graduated test measure having a capacity of at least three times the minimum specified quantity deviation of the measuring system to measure the discharge from the delivery hose of the road tanker under test.

Note: It may be necessary to use an intermediate receptacle to collect the volume discharged from the hose before measuring it in the graduated test measure in one or more measurements. ~~If the standard test measure used for the accuracy tests can be read accurately enough, this test could be started with the product level in the sight glass on a graduation mark and the volume of product released during this test could be measured by the rise in product.~~

B.3.4.4 Test procedure:

- a)1) Check that the hose closing device (e.g. a nozzle) is fitted with a device that prevents the draining of the hose (anti-drain device). ~~If the hose closing device is downstream of the anti-drain device (see ~~R-117~~OIML R 117-1, ~~clause~~ 2.13.6), the volume of product between these devices that will be released when the closing device is opened with the hose not being under pressure, will need to be considered if the hose dilation test fails.~~

Note: Where the hose closing device is downstream of the anti-drain device the ~~—~~volume between these devices should be less than the minimum specified ~~—~~quantity deviation (see ~~R-117~~OIML R 117-1, ~~clause~~ 2.13.6) and if the actual volume is ~~—~~unknown it will need to be determined and subtracted from the volume ~~—~~released during the hose dilation test if this test fails.

- b)2) Wet the test measure.
- c)3) Completely uncoil ~~the~~ hose from the hose reel or its normal storage position.
- 4) Deliver a quantity of product and abruptly stop the delivery by using the hose closing device.
- 5) Close the valve upstream of the hose; (the pump is still running, hose is still pressurized).

- ~~1) 6) Depressurize the hose by opening the hose closing valve. Measure the emergent liquid. Switch off the pump.~~
- ~~d) Close valves upstream of the hose and switch off the pump.~~
- ~~e) Coil the hose completely onto the hose reel or into its normal storage position.~~
- ~~f) Using the hose closing device, drain the hose into the test measure and determine the volume of product that is released.~~
- ~~g) 7) Check that the quantity released does not exceed the minimum specified quantity deviation (see 2.15) when not fitted with a hose reel, or twice the minimum specified quantity deviation when fitted with a hose reel. If the hose closing device is downstream of the anti-drain device and the volume in the test measure is greater than the allowed volume, determine the volume retained between the hose closing device and the anti-drain device and subtract this from the volume of product released in step 7.~~
- ~~h) 8) Repeat steps 2 to 8 twice, and calculate the mean value \bar{E}_v .~~
- ~~i) 9) Fill in the test report.~~

B.3.5 Complete emptying of the hose (empty hose measuring system only)

B.3.4.5 Object of the test

To determine the effect of the repeatability of the complete emptying of the hose by using additional devices or by gravity on the accuracy of the quantity indication.

B.3.4.6 Test procedure

The test shall be performed three times at a flowrate within the flowrate range of the measuring system. The test quantity shall be the minimum measured quantity. Information on the complete emptying procedure shall be fully documented in the test report.

- ~~1) 1) Wet and drain the test measure.~~
- ~~2) 2) Reset the indication of the CID.~~
- ~~3) 3) Deliver a quantity equal to the volume of the test measure.~~
- ~~4) 4) Read p_t and T_t at 50 % of the test volume.~~
- ~~5) 5) Empty the hose in accordance with manufacturer's instructions.~~
- ~~6) 6) Read V_i , V_s , and T_s .~~
- ~~7) 7) Calculate V_n and E_{vi} .~~
- ~~8) 8) Drain the test measure.~~
- ~~9) 9) Repeat steps 2 to 8 twice, and calculate the mean value \bar{E}_v .~~
- ~~10) 10) Fill in test report.~~

Annex E

Test procedures for measuring systems (MS) for milk, beer and other foaming potable liquids

(see ~~R 117~~R 117OIML R 117-1, ~~Section 5.6~~)

The tests in Annex E apply to measuring systems on road tankers and also to fixed measuring systems that are used for the reception or the delivery of milk, beer and other foaming potable liquids.

Note: “~~F~~ixed” is interpreted here as either fixed to a certain location or installed as a package which can be transported.

E.1 General ~~i~~Information

(As valid generally and not only for Annex E), the measuring systems (MS) consist of several constituent elements ~~which. These constituent elements~~ may or may not be subject to a separate type approval. According to ~~6.1.1 of OIML R 117~~6.1.1 of OIML R 117-1, ~~6.1.1~~ the constituent elements of an ~~MS-measuring system~~ shall comply with the relevant requirements.

The type approval of the ~~measuring system~~MS involves verifying that the constituent elements of the system, which have not been subject to separate type approvals, satisfy the applicable requirements.

Tests for carrying out the type approval of the ~~measuring system~~MS shall therefore be determined on the basis of the type approvals already granted for the constituent elements.

When none of the constituent elements has been subject to separate type approval, all tests provided in E.2 to E.7 shall be performed.

When the various constituent elements are all approved separately, it may be possible to replace type approval based on tests by type approval of drawings of the constituent elements. This possibility has to be considered cautiously and it may be appropriate ~~even if~~ in this case to perform an accuracy test on the complete ~~measuring system~~MS due to the possible influence of hydraulic conditions on the accuracy of the complete system.

Additionally, it shall be safeguarded for milk measuring systems, such that when the air elimination device has been approved separately, the tests have been performed with milk.)

Before conducting tests, it is necessary to perform the design examination of the MS by using the general check-list given in ~~R 117~~R 117OIML R 117-3 and the relevant points for such ~~MS~~ approval.

E.2 Tests for meter sensors, measuring devices and meters with mechanical indicating devices

For the electronic devices (calculator, conversion device, indicating device, associated devices) ~~tests~~ additional tests to E.2 apply, see ~~clause~~ E.3.

Tests are performed in accordance with ~~R 117~~R 117OIML R 117-2, ~~section~~ 5.

Tests shall be performed on a test bench, when the flowrate in the MS is not settable.

The tests consist of:

a) Accuracy tests:

Accuracy tests at metering conditions:

EUT for milk: tests shall be performed either with milk or with a liquid of a viscosity similar to milk (e.g. water);

~~M~~metering conditions: same as the typical operating conditions of the MS in use (i.e. temperature range approximately 1—15 °C, pressure range approximately 1—5 bar).

EUT for beer and other foaming liquids: tests shall be performed either with the liquid for the intended use or with a substitute with a viscosity similar to the liquid for the intended use (e.g. water);

metering conditions: same as the typical operating conditions of the MS in use (i.e. within the temperature and pressure range which is typical for the liquid for the intended use, e.g. for beer: temperature range approximately 1—15 °C, pressure range approximately 1—3 bar).

Accuracy tests at the limits of temperature, pressure, viscosity and density:

EUT for milk: tests are not required for an EUT intended for a milk MS which works under typical operating conditions as above (where the processing of milk ~~neither~~ allows ~~neither~~ high pressures nor temperatures ~~aside-outsidefrom~~ a small temperature range and the milk ~~has always~~ nearly always has the same density and viscosity).

—EUT for beer and other foaming liquids: tests are not required for an EUT intended for a MS which works under typical operating conditions as above (where the processing of the liquid ~~neither~~ allows ~~neither~~ high pressures nor temperatures ~~aside-outsidefrom~~ a small temperature range and the liquids concerned cover a small density/viscosity range).

Flow disturbance tests: see ~~R 117~~OIML R 117-1, 3.1.5.2

Note: EUT such as electromagnetic meters, ultrasonic meters, vortex meters, turbine meters (but not PD meters, Coriolis meter) are supposed to be sensitive to disturbances mainly caused by restricted space (meaning that e.g. bows, elbows are part of the pipe work upstream of the EUT thus leading to flow disturbances at the inlet of the EUT).

b) Endurance test;

c) Accuracy on the minimum measured quantity.

E.3 Tests for electronic devices <calculator, correction device, indicating device, associated devices>

Tests are performed in accordance with ~~R 117~~OIML R 117-2, ~~section~~ 6.

Note: Usually, the calculators are not manufactured directly for the special purpose of milk/beer MS. Therefore, care shall be taken that the legally relevant software of the calculator includes all functions and parameters which are necessary for the special measurement purpose, e.g. with milk MS the parameter <quantity required to fill the MS, colloquially “flood volume”> in case ~~that~~ the measured quantity is corrected automatically by this parameter.

When these electronic devices are connected to the meter sensors / measuring devices according to E.2, their compatibility with the meter sensors / measuring devices shall be established and declared by the manufacturers of the electronic devices.

E.4 Tests for air/gas elimination devices

E.4.1 Air elimination devices for MS for milk

Tests shall be performed with milk in the course of testing the complete MS according to E.6.1.

Note: Tests with water do not yield representative results for the air elimination device (the air elimination device is sensitive to the liquid used - cream and foam in the air elimination device may hamper its correct function, especially when the air elimination device contains mechanical parts, e.g. a float).

Note: Although other paragraphs of ~~R-117~~ ISO/IEC 17025:2014 may allow a separate type approval test of components, in the case of an air elimination device for MS for milk, separate tests are not feasible for the following reasons:

Receiving MS: The main purpose of the air elimination device is to ensure that under normal operating conditions of the MS (~~that is i.e.~~ under air intake at the start and end of the measurement according to ~~R-117~~ ISO/IEC 17025:2014 5.6.3, item 1 ~~and item 2~~) the MPE of the MS ($\pm 0.5\%$) is met. So this MPE can be tested only under conditions when the complete MS is present and when especially the hose and inlet line dimensions are as foreseen in the final version.

Furthermore, ~~R-117~~ ISO/IEC 17025:2014 5.6.3, item 2 requires that when the MS is equipped with hoses, which are designed to be coupled to the outlet of the supply tank, the gas elimination device shall also comply with the requirements in ~~R-117~~ ISO/IEC 17025:2014 2.10.1 during the entire measuring operation.

For such a design, sources of air during the whole measuring operation might possibly be leaking through couplings (or cracks in the coupled hoses or ~~and~~ similar effects) which could cause continuously and slightly mixed air. So, the air elimination device shall also be tested in the sense of a special gas extractor (~~R-117~~ ISO/IEC 17025:2014 2.10.9, second paragraph).- The gas extractor test of the air elimination device is already covered by the test in normal operation of the MS, when air pockets enter the MS at the start and at the end of a measurement; these air pockets are part of the rated operating conditions.

Receiving / delivering MS: To make the air elimination device operate properly under normal operating conditions, it is indispensable to embed it into the complex manufacturer specific control system belonging to the MS. So the air elimination device cannot be tested adequately ~~but except when with~~ all the parts and functions of the manufacturer specific control system are present ~~during at~~ the test.

For a separate test the following test pre-requisites ~~would be~~ are necessary:

- receiving MS: a suction system (vacuum) / pump system working under the same conditions as the MS for which the air elimination device is foreseen;
- receiving / delivering MS: a control system which can register the liquid level in the air elimination device and which can act upon it in the same way as the MS does;
- receiving / delivering MS: if applicable, regulating and non-return valves;
- receiving / delivering MS: in the case of MS equipped with an air elimination constructed as bubble sensors, a repeatable air injection system with variable injectors for variable bubble sizes and a settable and measured air injection rate;
- receiving / delivering MS: the testing facility needs to be operated with milk, and all standards as foreseen for testing the complete MS are necessary.

E.4.2 Gas elimination devices for MS for beer and other foaming potable liquids

Tests are performed ~~either~~ according to either a) or b).

- a) The EUT is tested in the course of testing the complete MS according to E.6.2.

Note: This is the preferable test, because such MS usually work under pressure, and the product can either be propelled by means of pressure in the supply tank or by a pump, and in some cases with a gas back pressure in the reception tank - which might influence the performance of the EUT; so by this test, the gas pressure influence can be better allowed for than by a separate test of the EUT.

- b) The EUT is tested separately according to ~~R 117~~ ISO/IEC 117-2, ~~section~~ 7.

Note: Section 7 states tests for different kinds of gas elimination devices (gas separators, gas extractors, special gas extractors). ~~E~~ each kind is characterized by ~~R 117~~ ISO/IEC 117-1, 2.10 according to its performance). The decision ~~of to fitting~~ a MS with a given kind of gas elimination device is based on an examination considering the worst conditions in which the MS could operate (e.g. in ~~the~~ case that ~~the~~ gas intake can only occur when the overground supply tank runs empty, the adequate kind of gas elimination device is a gas extractor).

The test liquid shall either be the same as for the intended use or of a viscosity which is similar to the liquid for the intended use, e.g. water.

The EUT shall comprise all parts defined by the manufacturer as being the gas elimination device.

In ~~the~~ case that for its proper operation the gas elimination device makes use of parts of the MS not defined by the manufacturer as being the gas elimination device, the test shall be performed together with these parts (e.g. a specific control system of the MS, into which the gas elimination device is embedded; ~~e.g. or~~ a shut off valve controlled by the gas elimination device which interrupts the flow during venting the gas elimination device).

The test report must state Q_{\max} and the upper and lower pressure of the gas elimination device.

Care shall be taken when installing the gas elimination device into the MS that ~~Q_{\max}~~ ~~Q_{\max}~~ and ~~P_{\max}~~ ~~P_{\max}~~ of the MS match with the rated operating conditions of the gas elimination device.

E.5 Tests for ancillary devices

The tests are performed in accordance with ~~R 117~~ ISO/IEC 117-2, ~~section~~ 8.

E.6 Additional tests on the complete MS

E.6.1 MS for ~~M~~ milk

General

The accuracy test ~~and the test of the special gas extractor function of the air elimination device~~ shall be performed either on the complete MS or on an installation which is representative for the complete MS.

Note: In order to achieve the required accuracy – especially for MS working at high ~~flow-rate~~ flowrate - many components form a complex system for the automatic control of the measurement procedure. So, any changes (additions or modifications) to the hardware or software of these components require an application for variant and a corresponding accuracy check as above.

Components of an installation which can be considered as representative for the complete MS:

- Pipe system: The dimensions of the suction lines shall be the same as and the spatial arrangement of the parts of the suction line upstream of the meter shall be similar to the complete MS.
- The air elimination device, its installation in the pipe system and its control unit shall be identical to the complete MS.
- The suction elements (such as pumps, ejectors) shall be of the same constructional and functional principle as in the complete MS, and the EUT shall be tested at the maximum capacity of the suction elements.

- The software (programs, parameters) of the control unit shall be identical to the complete MS. The SW-ID shall be registered.

All other components of the MS foreseen in the complete MS which may influence the performance of the MS (such as control valves being actuated by the control unit, pressure maintaining valves, a ventilation valve in an empty hose) shall be installed in the EUT as foreseen in the complete MS.

The meter sensor/measuring device/meter shall be installed in the EUT in a position as foreseen in the complete MS and according to the manufacturer's specification (straight pipes, flow straightening device, minimum back pressure, software setting/configuration, warm up time, etc.).

In the following of E.6.1 the EUT is always denoted as "MS", regardless of whether the test is performed on the complete MS or on an installation which is representative for the complete MS.

The accuracy test shall be performed with milk (ideally raw milk between 7 °C und 14 °C which causes little foam formation and creaming. ~~C; e~~are shall be taken that milk which has been pumped over- several times; still remains in a consistent stage. ~~E; f~~at shall be emulsified within the liquid and must not show a separation from the milk).

E.6.1.1 Accuracy test for a receiving MS for milk

The accuracy test is combined with the test of the air elimination device.

The accuracy test shall be performed at the maximum operational flowrate which is automatically set by the MS.

Note 1: Q_{\max} of the MS is considered to be the maximum ~~flow-rate~~flowrate attained during the test runs.

Note 2: Receiving MS cannot be tested by determining an error curve because the flowrate cannot be set, but is a function of the suction element.


Care shall be taken that the operational flowrate is the maximum attainable flowrate, and must not be reduced e.g. by the control unit or by the ratio of the vehicle's gear.

Before the start of each measurement test sufficient milk shall be passed through the MS to ensure that the MS is completely filled as foreseen.

At the start and finish of a measurement run, the requirement ~~R-117~~R-117OIML R 117-1, 5.6.2.4 must be fulfilled (settlement of constant level within the range defined by two marks on the sight glass). In the case that the MS measures the level in the constant level tank automatically before and after a measurement (e.g. by a dipstick) and corrects the received quantity according to the levels, 5.6.2.4 does not apply.

The measurement runs shall be performed without activating a sampling system.

The MS and the supply tank shall be located on level ground. ~~T; t~~he difference in height between the pump of the MS and the outlet valve of the supply tank shall not exceed 1 m up or down (see fig-~~ure~~ure, below).



Note: The receiving road tanker MS usually have a suction hose which may either be coupled to a suction pipe in order to suck off milk churns and other vessels of similar size or directly coupled to the outlet valve of a big supply tank. Receiving stationary MS usually have a suction hose which is directly coupled to the outlet valve of a supply tank.

- Test with suction pipe, at the operational flowrate of the MS; three independent and identical measurement runs. The measured quantity shall be such that a continuous flow at the maximum attainable flowrate during at least 1 min is established; anyway, this quantity shall not be less than 2 ~~xx~~ MMQ.
- Test without suction pipe, with the hose of the MS directly coupled to the supply tank (thus simulating a big supply tank), at the operational flowrate, three independent and identical measurement runs. The measured quantity shall be similar as above.

Note: Care shall be taken that the outlet valve of the supply tank is completely open. Otherwise cavitations may occur leading to the generation of air additional to the start and stop phase of the reception.

- Test of MMQ, with suction pipe, at the operational flowrate of the MS; three independent and identical measurement runs. Before this test a simulated measurement run with a quantity \approx MMQ shall be performed.

Each measurement run must fulfil the MPE.

Note: These tests cover the testing of the air elimination device under normal operating conditions. Contrary to other MS, where the entrance of air is beyond the normal operating conditions, the entrance of air described in [R-117R-117OIML R 117-1, 5.6.3, item 1](#), represents the normal working principle of a receiving MS for milk under rated operating conditions, for which the MPE applies. So, for receiving MS for milk where air / gas intake occurs often and is therefore considered to be a part of the normal operating conditions, the MPE equals the MPE of [R-117R-117OIML R 117-1, Table 2](#).

E.6.1.2 Test of the special gas extractor function of the air elimination device

Note: The test procedure below is analogous to the test procedures of [R-117OIML R 117-2, section-7](#) Testing procedures for gas elimination devices, with adjustments to the conditions of MS for milk.

Care shall be taken when choosing the type of the meter used for this test:

The efficiency of the air elimination device (expressed by the meter error $E_{(\text{with gas})} - E_{(\text{without gas})}$) can be determined appropriately only for meter types which count the air according to its real volume (such as PD meters). When the meter type does not count the real gas volume (which might be the case e.g. with electronic meters) then $E_{(\text{with gas})}$ is also affected by an unknown effect of the air on the meter. No problem exists when the air elimination device - tested by another meter type than a PD meter - complies and the MS is then approved for this combination under test.

The test shall be performed at the maximum operational ~~flow rate~~flowrate which is automatically set by the MS.

Note: Q_{\max} of the MS is considered to be the maximum ~~flow rate~~flowrate attained during the test runs.

Care shall be taken that the operational flowrate is the maximum attainable flowrate, and must not be reduced (e.g. by the control unit or by the ratio of the vehicle's gear).


The test quantity shall be at least the quantity delivered in one minute at the maximum attainable flowrate, Q_{\max} of the MS.

At the start and finish of each measurement run, the requirement of [R-117OIML R 117-1, 5.6.2.4](#) must be fulfilled (settlement of constant level within the range defined by two marks on the sight glass). In the case that the MS measures the level in the constant level tank automatically before and after a measurement (e.g. by a dipstick) and corrects the received quantity according to the levels, [R-117OIML R 117-1, Section 5.6.2.4](#) does not apply.

The measurement runs shall be performed without activating a sampling system.

The milk is supplied from the supply tank (prover). The MS and the supply tank shall be located on level ground; the difference in height between the pump of the MS and the outlet valve of the supply tank shall not exceed 1 m up or down (see figure below). The suction hose of the MS shall be directly coupled to the outlet valve of the supply tank.

The air is drawn in upstream of the air elimination device (either by injection or by suction) through the air control valve.



Test ~~i~~Installation

The volume of air continuously entering the liquid via the air intake is measured by a gas meter and isothermally converted to atmospheric pressure on the basis of the indication of a manometer fitted upstream of the gas meter. The conversion of the (corrected) volume indication $V_{\text{metered gas}}$ of the gas meter at the pressure p_t to the amount of added gas V_a at the atmospheric pressure $p_{\text{atmospheric}}$ is calculated by

$$V_a = \frac{V_{\text{metered gas}} \cdot (p_t + p_{\text{atmospheric}})}{p_{\text{atmospheric}}}$$

Note: The conversion is negligible in the case of sucked-in air.

The requirements of ~~R-117~~OIML R 117-1, ~~Sections~~ 2.10.1 and 2.10.9 shall be complied with under test conditions such that Q_{max} of the MS is reached when no air enters.

Test procedure

- 1) All measurements must start with the air inlet closed, and the hose empty up to the outlet valve of the supply tank. All measurements must finish with the air inlet closed and the supply tank and the hose empty.
- 2) Start each test run at Q_{max} of the MS. Then introduce air, regulating the air flow by the air inlet control valve. Follow the test steps below.
- 3) Calculate the error of the air elimination device by taking the error of the accuracy test into account.

Test steps

- 1) Set the entry of air to 0 %.
- 2) Vent the liquid pipework completely from entrapped air as foreseen for the accuracy test.
- 3) Make a test run at Q_{max} of the MS.
- 4) Read the liquid volume V_s of the liquid standard and calculate V_n . Then make the test run at Q_{max} by adding air of the required proportion. Start the test run with the air inlet closed. When Q_{max} is reached add air by regulating the air flow by the air inlet control valve.
- 5) Check the liquid and air ~~flow-rate~~flowrate together with the pressure values.
- 6) Stop the flow of air shortly before the supply tank ~~gets~~becomes empty.
- 7) Read the volume V_i indicated by the liquid meter and calculate V_a .
- 8) Calculate the ratio of V_a/V_n and the relative meter error $E_{\text{vi(with gas)}} = (V_i - V_n)/V_n$ and determine the difference between $E_{\text{vi(with gas)}}$ and $E_{\text{vi(without gas)}}$ as the relative error of the gas elimination device due to the added air.
- 9) Repeat steps 4—8 by increasing the air/liquid ratio successively up to 5 %.

~~E.6.1.2~~E.6.1.3 2 Accuracy test for delivering MS for milk

Note: Contrary to receiving MS for milk the accuracy test is not combined with the test of the air elimination device. ~~T;~~the test of the air elimination device is described in C.6.1.3.

In the case of an empty hose MS, the MS and the receiver tank shall be located on such a level that the empty hose can be completely emptied.

Before the start of the measurement tests sufficient liquid shall be passed through the MS to ensure that the MS is completely filled.

The measurement runs shall be performed without activating a sampling system.

- Test at Q_{\min} , Q_{\max} and at an intermediate flowrate.

Note: Q_{\max} of the MS is considered to be the maximum ~~flow-rate~~flowrate attained during the test runs.

Care shall be taken that the operational flowrate is the maximum attainable flowrate, and must not be reduced e.g. by the control unit.

The measured quantity shall be such that a continuous flow at the maximum attainable flowrate during at least 1 min is established for all ~~flow-rate~~flowrates tested. This quantity shall not be less than 2 ~~×~~ MMQ.

- Test of MMQ, at any ~~flow-rate~~flowrate between Q_{\min} ~~Q_{\min}~~ and Q_{\max} ~~Q_{\max}~~ , three independent and identical measurement runs.

Each measurement run must fulfil the MPE.

~~E.6.1.3~~E.6.1.4 **3**Test of the air elimination device for delivering MS for milk

Note 1: Contrary to receiving MS for milk for which requirements concerning the design and the extent of tests of the air elimination device are well defined (see ~~R-117~~R-117OIML R 117-1, 5.6), adequate requirements for delivering MS for milk are missing there. So for delivering MS for milk, the considerations on the supply conditions (leading to the right choice of the kind of the gas elimination device) refer to ~~R-117~~R-117OIML R 117-1, 2.10.2 (pumped flow) and ~~R-117~~R-117OIML R 117-1, 2.10.3 (non-pumped flow), and the extent of tests refers to ~~R-117~~R-117OIML R 117-1, 2.10.8 (gas separator) and 2.10.9 (gas extractor, special gas extractor).

Note 2: The test procedures below are analogous to the test procedures of ~~R-117~~R-117OIML R 117-2, ~~section-7-~~ “Testing procedures for gas elimination devices”, with adjustments to the conditions of MS for milk.

Tests on gas elimination devices should be carried out for ~~flow-rate~~flowrates up to Q_{\max} ~~Q_{\max}~~ of the MS.

The test quantity shall be at least the quantity delivered in one minute at the maximum attainable flowrate Q_{\max} ~~Q_{\max}~~ of the MS.

The test shall be performed twice; from the two test runs the mean error value \bar{E}_v shall be calculated.

~~E.6.1.3.1~~E.6.1.4.1 **3**Tests on gas separators

The milk is supplied from the supply tank of the MS. The air is drawn in upstream of the gas separator (either by injection or by suction) through an air inlet control valve.

The volume of air continuously entering the liquid is measured by a gas meter and isothermally converted to atmospheric pressure on the basis of the indication of a manometer fitted upstream of the gas meter. The conversion of the (corrected) volume indication $V_{\text{metered gas}}$ of the gas meter at the pressure p_t to the amount of added gas V_a at the atmospheric pressure $p_{\text{atmospheric}}$ is calculated by

$$V_a = \frac{V_{\text{metered gas}} \cdot (p_t + p_{\text{atmospheric}})}{p_{\text{atmospheric}}}$$

Note: The conversion is negligible in the case of sucked-in air.

As required by ~~R-117~~R-117OIML R 117-1, 2.10.8, it is not necessary to use a gas meter if the gas separator is capable of separating and eliminating the air introduced in any proportion,.

The requirements of ~~R-117~~R-117OIML R 117-1, 2.10.1 and 2.10.8 shall be complied with under test conditions such that Q_{\max} ~~Q_{\max}~~ of the MS is reached when no air enters.

Test procedure

- All measurements must start with the air inlet closed, and the hose full and pressurized. All measurements must finish with the air inlet closed and the hose pressurized.
- Determine the error curve of the meter from Q_{min} ~~Q_{min}~~ to Q_{max} ~~Q_{max}~~ of the MS.
- Start each test run at Q_{max} ~~Q_{max}~~ of the MS. Then introduce air, regulating the air flow by using the air inlet control valve. Follow the test steps below.
- If there is no liquid flow for more than 10 seconds, close the air inlet and terminate the test run until the test quantity of the liquid is reached.
- Measurement results gained below Q_{min} ~~Q_{min}~~ shall be disregarded.
- Calculate the error of the gas separator by taking the error curve of the meter into account.

Test steps

- X.51) Set the entry of air to 0 %.
- X.62) Vent the liquid pipework completely from entrapped air.
- 1)3) Make a test run at Q_{max} ~~Q_{max}~~ of the MS.
- X.74) Make the test run at Q_{max} ~~Q_{max}~~ by adding air of the required proportion. Start the test run with the air inlet closed. When Q_{max} ~~Q_{max}~~ is reached add air by regulating the air flow by the air inlet control valve.
- X.85) Check the liquid and air ~~flow-rate~~ flowrate together with the pressure values.
- 2)6) Stop the flow of air and liquid when the test quantity of the liquid is reached.
- 3)7) Read the liquid volume V_s of the liquid standard and the volume V_i indicated by the liquid meter and calculate V_n .
- X.98) Calculate the ratio of V_a/V_n and the relative meter error $E_{vi(with\ gas)} = (V_i - V_n)/V_n$ and determine the difference between $E_{vi(with\ gas)}$ and $E_{vi(without\ gas)}$ as the relative error of the gas elimination device due to the added air.
- 4)9) Repeat step 4—8 by increasing the air/liquid ratio. This procedure shall be terminated under the condition of either a) or b):
 - a) when it covers the entire range of air/liquid ratio V_a/V_n
 - b) when the discharge stops automatically.

10.1.1.18.5.3.1 3 Tests on gas extractors

An air pocket is created (either by emptying the liquid pipework upstream of the gas extractor or by emptying the gas extractor itself) of a volume (under atmospheric pressure) equal to the MMQ of the MS. The other parts of the liquid pipework upstream of the meter must be kept full.

This gas pocket is added to the liquid during the delivery.

When the test is performed by filling up the supply tank with the test quantity and after the delivery of the liquid the supply tank becomes completely empty (residual discharge), the volume of the air pocket is deemed to be of the required volume.

Perform the measurements for pumped flow and/or for not-pumped flow, whatever is applicable.

Test steps

- 1) Vent the liquid pipework completely from entrapped air.
- 1)2) Make a test run by setting the MS to Q_{max} ~~Q_{max}~~ and add the air pocket to the liquid.

2)3) For adding the air pocket during the delivery: After the gas extractor had acted upon the air pocket, the ~~flow-rate~~ flowrate will resume ~~Q_{\max}~~ Q_{\max} ; continue the delivery at ~~Q_{\max}~~ Q_{\max} and stop it by the delivery valve of the MS, as soon as the test quantity of the liquid is reached.

For a residual discharge: After the gas extractor had acted upon the air pocket, the flow is either stopped automatically or the delivery valve of the MS is closed manually when the ~~flow-rate~~ flowrate is zero for more than 30 s.

3)4) Read the standard volume V_s and the volume V_i indicated by the meter. Calculate V_n .

Calculate the meter error $E_{vi(\text{with gas})} = (V_i - V_n)$ and determine the difference between the meter error $E_{vi(\text{with gas})}$ and $E_{vi(\text{without gas})}$ as the absolute error of the air elimination device due to the added air.

Note: For a gas extractor, the error limits of ~~R 117~~ QIML R 117-1, 2.10.1 apply: The effect due to the influence of air or gases on the measuring result must not exceed 1 % of quantity delivered (but need not be less than MMQ).

For this test, air is not added continuously, but only once during a delivery. But the error limit of $\leq 1\%$ of quantity delivered means that the test volume can be manipulated to a larger volume that enables this test to be successful when air is introduced only once.

In order to cope with that problem, the test volume should be related to the worst case, i.e. to the delivery of the MMQ (with the applicable error limit for the MMQ of 1 % of the MMQ). ~~F;~~ but for practical reasons it is preferable to deliver a test quantity \geq MMQ; in this case the determination of the difference between the meter error $E_{vi(\text{with gas})}$ and $E_{vi(\text{without gas})}$ shall be related to the delivery of MMQ by taking into account the absolute (and not the relative) errors. The difference then must be $\leq 1\%$ of MMQ.

~~10.1.1.28.5.3.2~~ 3 Tests of special gas extractors

- Special gas extractors not intended for MS on road tankers:

- ~~b)0~~ Test of the gas separator function: see E.6.1.~~43.1~~;

- Test of the gas extractor function: see E.6.1.~~43.2~~.

Special gas extractors intended for MS on road tankers:

- Test of the gas separator function: The test of the gas extractor function as stated below gives sufficient evidence that the special gas extractor meets the requirements of ~~R 117~~ QIML R 117-1, 2.10.9, second paragraph.
- Test of the gas extractor function: according to E.6.1.~~43.2~~ by residual discharge. For MS with empty hoses the test of the residual discharge shall be carried out such that the delivery to an underground reception tank is simulated: either the reception tank is placed approx. 3 m beneath the level of the empty hose valve or an under-pressure of approx. ~~0.5~~ 3 bar is generated in the hose (e.g. by an acceleration pump). Care shall be taken that the meter remains completely filled with liquid during the test and that the pressure directly behind the meter does not fall below atmospheric pressure.
- Measurement procedures (gravimetric or volumetric):

1a. Volumetric procedure by receiving the liquid from a standard capacity measure

Each measurement run comprises:

- ~~—~~ Fill the standard capacity measure, wait until entrained air has been released from the milk and then read V_s , T_s .
- Reset the indication device of the meter to zero.
- ~~—~~ Start the reception. In the case of a suction pipe suck from the bottom of the supply tank and in the case of a hose coupled to the outlet of a supply tank open the outlet valve.

- Suck until the measure is empty and the MS finishes the reception automatically.
- ~~Read~~ V_i and calculate V_n and E_{vi} .

Note 1: V_n is the volume of the test measure at temperature when reading is taken.

Usually, the differences between the temperature at the standard capacity measure and the temperature at the MS are small so that conversion can be neglected, especially when considering the small coefficient of expansion of milk compared e.g. with that of hydrocarbons.

Note 2: This procedure covers the testing of the air elimination device under normal operating conditions.

1b. Volumetric procedure by delivering the liquid into a standard capacity measure

Each measurement run comprises:

- Wait until entrained air has been released from the milk in the supply tank.
- Reset the indication device of the meter to zero.
- Start the delivery.
- Stop the delivery until the measure is full.
- Read V_s , T_s , V_i and calculate V_n and E_{vi} .

Note: V_n is the volume as above.

2a. Gravimetric procedure by receiving the liquid from a tank on a balance

- The weighing instrument (balance) should be of a suitable capacity and a suitable verification scale interval.

Note: A scale interval corresponding to a quantity not greater than 1/10 of the MPE of the MS at the quantity tested is considered as suitable.

- When determining the suitability of the weighing instrument consider situations where the tare weight of the vessel is likely to vary (e.g. fuel consumption in a vehicle which forms part of the tare weight of the vessel).
- Changeover points can be used to increase the indicating resolution of the weighing instrument.

Note: “eChangeover points” means the point at which a digital indication changes from one scale interval to the next scale interval. This is done by adding weights equal to not more than 10% of the value of a scale interval to the balance to make the indication increase by 1 digit and then determining the true value of the indication to 10% of a scale interval.

Each measurement run comprises:

- Fill the tank, wait until entrained air has been released from the milk and then draw a sample of the milk (without any entrained air) from the tank, determine its density $\rho(T_s')$ and calculate $\rho(T_s)$ from $\rho(T_s')$ (take an approximate volume expansion factor of water = $200 \cdot 10^{-6} \text{ } ^\circ\text{C}^{-1}$):

$$\rho(T_s) = \rho(T_s') + 200 \cdot 10^{-6} \cdot \rho(T_s') \cdot (T_s' - T_s)$$

Determine the gross weight W_{gross} of the tank and milk and T_s

Note: When the hose is coupled to the tank and this influences the reading of the balance, the hose has to be uncoupled before reading.

- Reset the indication device of the meter to zero.
- Start the pump. In the case of a suction pipe suck from the bottom of the supply tank and in the case of a hose coupled to the outlet of a supply tank open the outlet valve.
- Suck until the tank is empty and the MS finishes the reception automatically.

- Read V_i and the weight of the empty tank as indicated by the balance.
- From the gross weight and weight of the empty tank determine the net weight of the milk after correcting for air buoyancy (assume air density as 0.0012 kg/L and enter this value into the formula in the appropriate units) and from $\rho(T_s)$ calculate V_n and E_{vi} :

$$V_n = (W_{\text{gross}} - W_{\text{net}}) / \rho(T_s) \times (1 + 0.0012 / \rho(T_s))$$

Note: This procedure covers the testing of the air elimination device under normal operating conditions.

2b. Gravimetric procedure by delivering the liquid into a tank on a balance

- The weighing instrument (balance) should be of a suitable capacity and a suitable verification scale interval.

Note: A scale interval corresponding to a quantity not greater than 1/10 of the MPE of the MS at the quantity tested is considered as suitable.

- When determining the suitability of the weighing instrument consider situations where the tare weight of the vessel is likely to vary (e.g. fuel consumption in a vehicle which forms part of the tare weight of the vessel).
- Changeover points can be used to increase the indicating resolution of the weighing instrument.

Note: “eChangeover points” means the point at which a digital indication changes from one scale interval to the next scale interval. This is done by adding weights equal to not more than 10% of the value of a scale interval to the balance to make the indication increase by 1 digit and then determining the true value of the indication to 10% of a scale interval.

Each measurement run comprises:

- Wait until entrained air has been released from the milk in the supply tank.

Determine the net weight W_{net} of the reception tank on the balance.

Note: When the hose is coupled to the tank and this influences the reading of the balance, the hose has to be uncoupled before reading.

- Reset the indication device of the meter to zero.
- Start the delivery.
- Stop the delivery until the desired quantity is reached.
- Read V_i and the weight W_{gross} of the full reception tank as indicated by the balance.
- Draw a sample of the milk (without any entrained air) from the reception tank, determine its density $\rho(T_s')$ and calculate $\rho(T_s)$ from $\rho(T_s')$ (take an approximate volume expansion factor of water = $200.10^{-6} \text{ } ^\circ\text{C}^{-1}$):

$$\rho(T_s) = \rho(T_s') + 200.10^{-6} \cdot \rho(T_s') \times (T_s' - T_s)$$

- From the gross weight and weight of the empty tank determine the net weight of the milk after correcting for air buoyancy (assume air density as 0.0012 kg/L and enter this value into the formula in the appropriate units) and from $\rho(T_s)$ calculate V_n and E_{vi} :

$$V_n = (W_{\text{gross}} - W_{\text{net}}) / \rho(T_s) \times (1 + 0.0012 / \rho(T_s))$$

Note: This procedure covers the testing of the air elimination device under normal operating conditions.

E.1.1.1

E.1.1.2

~~E.1.1.3~~E.1.1.1 ~~4~~In a**Additionally to the tests of E.6.1.1 – E.6.1.43, the following shall be checked/examined:**

- Check that it is impossible during a measurement to reset the indicating device to zero (that means when the suction process comes to an end, the indicating device cannot be reset to zero before the constant level has been reached). When the level is registered automatically (e.g. by an electronic dip stick) check that resetting of the indicating device to zero is not possible before the level is registered, and that the level remains constant after registration.
- Check that there are no means by which liquid can be diverted during its passage from the supply tank to the receiving tank without being measured by the MS. A manually controlled outlet that may be opened for purging or draining the MS is permissible, but effective means shall be provided to prevent passage of liquid through any outlet during normal operation of the MS.
- Examine/test the sampling system (if provided).

Although the sampling system is not under metrological control, it shall be checked to ensure that it does not interfere with the metrological characteristics of the MS.

If documentary evidence is given that this is the case, no test is necessary; if not, a test shall be performed by activating the sampling system during a measurement run. The measurement must fulfil the MPE.

~~E.6.1.4~~E.6.1.5 **5Test of the volume required to fill the measuring system (colloquially “flood volume”, “dry start priming volume”) (~~R-117~~R-117OIML R 117-1, Section 5.6.2.7)**

This test is performed in the course of the initial verification and need not be performed in the course of a subsequent verification provided that no parts of the MS have been changed since the initial verification which could affect the flood volume.

Test procedure:

Empty the MS completely, without the pump running. The milk is received from a standard capacity measure with volume V_n . The difference between the volume V_n and the indication of the meter, corrected by the meter error, is the searched volume required to fill the MS. This measurement shall be done twice and the result taken as the mean value.

E.6.2 MS for beer and other foaming liquids

E.6.2.1 Accuracy test

The tests shall be performed in the delivery mode for systems only intended for delivery. -Additional tests are given for systems that will also be used for receiving liquid.

Note: Although in general the MS are foreseen for the delivery of liquids, they may also be designed for the reception of liquids.

The test shall be performed either with the liquid for the intended use or with a substitute of a similar characteristic (when the liquid for the intended use contains carbonic acid then the substitute shall also contain carbonic acid to a similar extent).

Temperature of the liquid: within the limits of the temperature range of the MS.

Because MS for beer and other foaming liquids are full hose systems, the EUT and the standard (balance / standard capacity measure) may be located on any level.

Before the start of the measurements, sufficient liquid shall be passed through the MS to ensure that the MS is completely filled.

- Test at Q_{\min} , ~~Q_{\max}~~ and at 2 intermediate flowrates evenly spaced over the flowrate range.

Note: ~~Q_{\max}~~ ~~Q_{\min}~~ of the MS is considered to be the maximum ~~flow rate~~ flowrate attained during the test runs.

The measured quantity shall be such that a continuous flow at the maximum attainable flowrate during at least 1 min is established for all ~~flow rate~~ flowrates tested. This quantity shall not be less than 2 ~~×~~ MMQ.

Note: ~~R 117~~ ~~R 117~~ OIML R 117-1, 2.3.3.3 requires for MS a ratio of ~~Q_{\max}~~ ~~Q_{\min}~~ : ~~Q_{\min}~~ ~~Q_{\min}~~ $\geq 5:1$ (this ratio is defined by ~~Q_{\min}~~ ~~Q_{\min}~~ of the meter and by ~~Q_{\max}~~ ~~Q_{\max}~~ of the MS). This ratio may be less, but the MS shall be fitted with an automatic checking device to detect when the flowrate of the liquid to be measured is outside the restricted flowrate range. In the case of MS for beer and other foaming liquids, for quality reasons of the delivered liquids, it is to keep ~~Q_{\max}~~ should be maintained ~~Q_{\max}~~ low (flow speed below 2 m/s in order to avoid a big shear force at the pipe surface which deteriorates the quality of the liquid), whereas the nominal size of the meter shall be relatively high (consequently ~~Q_{\min}~~ ~~Q_{\min}~~ of the meter is adequately high), so that the actual ratio ~~Q_{\max}~~ ~~Q_{\max}~~ : ~~Q_{\min}~~ ~~Q_{\min}~~ for such MS may be below 5:1.

- Test of MMQ, at any ~~flow rate~~ flowrate between ~~Q_{\min}~~ ~~Q_{\min}~~ and ~~Q_{\max}~~ ~~Q_{\max}~~ ; three independent and identical measurement runs.
- In the case where the MS is intended also for the reception of liquid and the reception procedure is under metrological control:

Note: Usually, the pipework for the reception is designed and can be operated such that the pump of the MS is able to suck liquid from a supply tank over the delivery hose and is able to propel it over the gas elimination device and the meter back to the supply tank of the MS. In order to prevent oxidation of the liquid, it is the intended concept of such MS that during the reception no parts of the pipework run empty.

A test additional to the test of the first bullet at an intermediate flowrate shall be performed, with two independent and identical measurement runs. The measured quantity shall be such that a continuous flow at the maximum attainable flowrate during at least 1 min is established. This quantity shall not be less than 2 ~~×~~ MMQ.

The MS shall be completely filled before the start of the test and the reception shall be performed by draining a known volume from a supply tank (standard capacity measure or tank on a balance), until the desired quantity is reached without ~~that~~ gases or air are being introduced from the supply tank into the MS.

Each measurement ~~must~~ shall fulfil the MPE.

Measurement procedures (gravimetric or volumetric) to deliver:

1) **Gravimetric procedure** by delivering the liquid into a reception tank on a balance.

- The weighing instrument (balance) should have a suitable capacity and a suitable scale interval.

Note: A scale interval corresponding to a quantity not greater than 1/10 of the MPE of the MS at the quantity tested is considered as suitable.

- When determining the suitability of the weighing instrument, consider situations where the tare weight of the vessel is likely to vary (e.g. fuel consumption in a vehicle which forms part of the tare weight of the vessel).
- Changeover points can be used to increase the indicating resolution of the weighing instrument.

Note: “Changeover points” means the point at which a digital indication changes from one scale interval to the next scale interval. This is done by adding weights equal to not more than 10% of the value of a scale interval to the balance to make the indication increase by 1 digit and then determining the true value of the indication to 10% of a scale interval.

Each measurement run comprises:

- Perform the delivery with the hose uncoiled from the reel, if present.
- Fill the delivery hose up to the reception valve of the reception tank.

The reception tank shall be ~~thus~~ prepared such that the necessary back pressure representative for the normal use of such a MS is established in the tank before the delivery starts. ~~D;~~ during the delivery the pressure supply shall be switched off, and no pressure shall be released.

- Read the indication of the weight of the tank on the balance.

Note: When the hose is coupled to the tank and this influences the reading of the balance, the hose has to be uncoupled before reading. By doing so, the pipe section between the coupling mechanism of the hose and the reception valve of the tank runs empty. Thus, at the start of the delivery a liquid volume corresponding to this pipe section passes the meter without being registered by the balance. This volume has to be subtracted from the indication of the meter.

- Keep the delivery valve closed and start the pump / the pressurizing system (hose becomes pressurized), then reset the indication device of the meter to zero.
- Start the delivery and fill the tank without pressure release.

~~Please Note~~ that any gas quantity released from or added to the tank during a run contributes to the mass measurement by the balance. So if for any reasons de-pressurizing/pressurizing the tank is necessary during a run (e.g. because the pressure of the pump does not overcome the back pressure in the tank, the back pressure is too low so that the pressure control of the measuring system stops the delivery, etc.), make the corresponding correction for that subtracted/added quantity of gas. The correction is calculated by considering that the respective mass of gas in the reception tank at the pressure P (reading the manometer of the reception tank) is given by:

the volume of gas in the tank:

$$V_{\text{air/gas in the tank}} = V_{\text{tank}} - V_{\text{liquid in the tank}}$$

and the gas density in the tank at pressure P:

$$\rho_{\text{gas}}(P) = \rho_{\text{gas}}(P_{\text{atmosphere in bar}}) \times^* (\text{reading of tank manometer in bar} + 1)$$

$$\rho_{\text{CO}_2} (15^\circ\text{C}, 1 \text{ bar}) \approx 1.8 \text{ kg/m}^3$$

- During the delivery determine the mean liquid temperature T_s (using a reference standard thermometer with a measurement uncertainty $\leq \pm 0.2^\circ\text{C}$).

Note: The liquid temperature can either be determined by an inline temperature sensor or by drawing a sample (e.g. from a vent pipe) into a Dewar vessel. Care shall be taken that the determined temperature is representative for the mean temperature of the metered liquid. In the case that the sample is diverted from the metered liquid, correct the metered liquid adequately for the diverted quantity.

During the delivery draw a sample of the liquid and determine its density $\rho(T_s')$ and calculate $\rho(T_s)$ from $\rho(T_s')$ (take an approximate volume expansion factor of water = $200 \cdot 10^{-6} \text{ }^\circ\text{C}^{-1}$):

$$\rho(T_s) = \rho(T_s') + 200 \cdot 10^{-6} \cdot \rho(T_s') \times^* (T_s' - T_s)$$

Note 1: In the case that the sample is diverted from the metered liquid, correct the metered liquid adequately for the diverted quantity.

Note 2: Because the liquid is carbonated, care has to be taken that the density determination covers the liquid together with its dissolved gas. -The density of the liquid together with its dissolved gas can be determined, e.g.

- by diverting the sample into a glass vessel under pressure, which contains the densitometer (during the density determination the gas remains dissolved).

- by diverting the sample into a volume measure under pressure. Determine the volume and the mass of the liquid, and from that calculate the density of the carbonated liquid~~;~~.
- ~~s~~SStop the delivery by the closure of the delivery valve (hose still pressurized), read V_i and then switch off the pump / the pressurizing system~~;~~.
- ~~r~~RRead the gross weight of the balance (weight of tank and liquid).

Note 3: When the hose is coupled to the tank and this influences the reading of the balance, then uncouple the hose while reading.

From the gross weight and weight of the tank and from $\rho(T_s)$ calculate V_n and E_{vi} .

Do not correct for buoyancy (no gas was displaced from the tank).

Note: Filling the tank with liquid increases the gas pressure in the tank thus increasing the back pressure, which decreases the flowrate. From start to finish the flowrate Q passes a spectrum and so do the errors of the meter. In order to avoid that the resulting (mean) error E_{vi} is a combination of errors $> \text{MPE}$ and $< \text{MPE}$, Q has to be kept relatively constant during the delivery. This can be achieved by de-pressurizing the tank after each test run and by emptying the tank after one or several test runs.

2) Volumetric procedure to receive the liquid from~~by delivering the liquid into~~ a pressurized (closed) standard capacity measure.

Each measurement run comprises:

- ~~p~~PPerform the delivery with the hose uncoiled from the reel, if present~~;~~.
- ~~w~~Wet and drain the standard capacity measure. Adhere to the correct drainage time of the measure used~~;~~.
- ~~f~~Fill the delivery hose up to the reception valve of the measure~~;~~.
- ~~k~~KKeep the delivery valve closed and start the pump/pressurizing system (hose becomes pressurized), then reset the indication device of the meter to zero~~;~~.
- ~~s~~SStart the delivery and fill the measure without pressure release~~;~~.
- ~~s~~SStop the delivery by the closure of the delivery valve (hose still pressurized), read V_i and then switch off the pump/pressurizing system~~;~~.
- ~~R~~Read V_s , T_s and p_s and calculate V_n and E_{vi} .

Note: MS for beer and other foaming liquids usually work under low pressure. A volume correction of the measure according to the pressure P_s has to be performed only in the case when the influence of the pressure on the volume of the measure exceeds 1/10 of the MPE.

Measurement procedures (gravimetric or volumetric) to receive:

Gravimetric procedure to receive the liquid from a delivery tank on a balance~~;~~.

For the suitable capacity, the suitable scale interval and the changeover points see gravimetric procedure to deliver.

Each measurement run comprises:

- ~~p~~PPerform the reception with the hose of the MS uncoiled from the reel, if present~~;~~.
- ~~F~~Fill the hose of the MS up to the delivery valve of the delivery tank.

The delivery tank shall be ~~thus~~ prepared such that the necessary back pressure representative for the normal use of such a MS is established in the tank before the reception starts. ~~D;~~ during the reception the pressure supply shall be switched off, and no pressure shall be released.

The delivery tank must be filled up with sufficient liquid so that during the reception no gas is sucked from the tank.

- Read the gross weight on the balance.

Note: When the coupling of the hose (to the tank) influences the reading of the balance, the hose has to be uncoupled before reading. But by doing so, the pipe section between the coupling mechanism of the hose and the delivery valve of the tank runs empty. Thus, at the reception a liquid volume corresponding to this emptied pipe section is missing at the meter but which had been registered by the balance. This volume has to be added to the indication of the meter.

- ~~R~~eset the meter to zero, open the delivery valve of the delivery tank and then start the suction;
- ~~e~~Empy the tank without pressure release.

~~Please Note~~ that any gas quantity released from or added to the tank during a run contributes to the mass measurement by the balance. So if for any reasons de-pressurizing/pressurizing the tank is necessary during a run, make the corresponding correction for that subtracted/added quantity of gas. The correction is calculated by considering that the respective mass of gas in the reception tank at the pressure P (reading the manometer of the reception tank) is given by

- the volume of gas in the tank:

$$V_{\text{air/gas in the tank}} = V_{\text{tank}} - V_{\text{liquid in the tank}}$$

- and the gas density in the tank at pressure P :

$$\rho_{\text{gas}}(P) = \rho_{\text{gas}}(P_{\text{atmosphere in bar}}) \times \frac{P}{P_{\text{atmosphere}}} \quad (\text{reading of tank manometer in bar} + 1)$$

$$\rho_{\text{CO}_2} (15^\circ\text{C}, 1 \text{ bar}) \approx 1.8 \text{ kg/m}^3$$

- ~~D~~during the reception, determine the mean liquid temperature T_s as described for the gravimetric procedure by delivering;
- during the reception, draw a sample of the liquid and determine its density $\rho(T_s)$ and calculate $\rho(T_s)$ from $\rho(T_s)$ as described for the gravimetric procedure by delivering.
- ~~S~~stop the reception by switching off the suction and then close the delivery valve; read V_i ;
- ~~R~~read the net weight of the balance;

Note: When the hose is coupled to the tank and this influences the reading of the balance, then uncouple the hose while reading.

- from the gross weight, net weight and $\rho(T_s)$ calculate V_n and E_{vi} .

Do not correct for buoyancy (no gas was displaced from nor added to the tank).

Volumetric procedure to receive the liquid from a pressurized (closed) standard capacity measure:

This procedure is only applicable for standard capacity measures which allow the delivery of the required test volume without running empty (e.g. standard capacity measures with a level tube).

Each measurement run comprises:

- ~~p~~Perform the reception with the hose of the MS uncoiled from the reel, if present;
- ~~F~~Fill the standard capacity measure with sufficient liquid so that during the reception no gas is sucked from the standard capacity measure.

The standard capacity measure shall be ~~thus~~ prepared such that the necessary back pressure representative for the normal use of the MS under test is established in the standard capacity measure during the reception.

Read the upper volume V_s of the standard capacity measure and T_s .

- ~~—~~ Fill the delivery hose up to the delivery valve of the measure;

- ~~r~~Reset the meter to zero, open the delivery valve and then start the suction;
- ~~s~~Stop the delivery by switching off the suction, then close the delivery valve and read the lower volume V_s of the standard capacity measure;
- ~~f~~From the upper and lower volume V_s and from T_s calculate V_n and E_{vi} .

Note: MS for beer and other foaming liquids usually work under low pressure. A volume correction of the measure according to the pressure has to be performed only in the case when the influence of the pressure on the volume of the measure exceeds 1/10 of the MPE.

~~10.1.1.38.5.3.3~~ Test of the gas elimination device

This test consists of a residual discharge from a supply tank (gas pocket test).

The supply tank (for road tankers: a compartment of a road tanker) is filled with the test quantity and then completely emptied until the delivery is interrupted by the gas elimination device.

Note: For this test, the volumetric method is less appropriate than the gravimetric method, because the volumetric method requires the actual quantity delivered at the end of the test to be within the readable range of the standard capacity measure.

The test shall be performed in the delivery mode.

~~For To evaluating~~ correctly evaluate the efficiency of the gas elimination device, adequate test conditions have to be established: the back pressure in the receiving tank shall be low (≈ 0.2 bar) and the pressure of the CO_2 -atmosphere in the supply tank shall be the same as in normal operation (> 0.5 bar).

The test shall be performed twice at the maximum attainable flowrate Q_{\max} of the MS; from the two test runs the mean error value \bar{E}_v shall be calculated.

The test quantity shall be at least the quantity delivered in one minute at the maximum attainable flowrate Q_{\max} .

Note: Gas is not added continuously (and the pressure - by design of such MS - will neither fall below atmospheric nor below the saturated vapor pressure of the liquid), but only once during a residual discharge, when the supply tank becomes empty and gas pockets are introduced into the pipework (see ~~R 117~~OIML R 117-1, 2.10.2).

So the gas elimination device has to be tested as a gas extractor (gas pocket test), for which the error limits of ~~R 117~~OIML R 117-1, 2.10.1 apply: The effect due to the influence of air or gases on the measuring result must not exceed 1 % of quantity delivered (but need not be less than MMQ).

But this error limit of ≤ 1 % of quantity delivered means that the test volume can be manipulated to a larger volume that enables this test to be successful when gas is introduced only once. ~~I;~~ in order to cope with that problem, the test volume shall be related to the worst case, i.e. to the delivery of the MMQ (with the applicable error limit for the MMQ of 1 % of the MMQ).

For practical reasons it is more feasible to deliver a test quantity $\geq \text{MMQ}$. ~~I;~~ in this case the determination of the difference between the meter error $E_{vi(\text{with gas})}$ and $E_{vi(\text{without gas})}$ shall be related to the delivery of MMQ by taking into account the absolute (and not the relative) errors. The difference then must be ≤ 1 % of MMQ.

The test procedure is the same as for the accuracy test, with the exception that the delivery is interrupted by the gas elimination device. ~~I;~~ in the case that a continuation of the delivery is possible (e.g. by a manual re-start of the pump), the delivery shall be continued until gas is clearly visible in the sight glass and until any re-start is impossible. The delivery is stopped by the closure of the delivery valve.

Note: Because such MS usually control the delivery procedure automatically, they may interrupt the flow for different reasons (e.g. when the gas elimination device registers gas, ~~e.g. or~~ -when a low ~~flow~~ rate/flowrate is registered over a certain period due to a high back pressure in the reception tank).

Therefore care shall be taken that such an interruption is not always interpreted as the response of the gas elimination device to the entrance of gas and therefore as the end of the delivery.

E.7 ~~E.7~~ Hose variation (see ~~R-117~~OIML R 117-1, 2.15)

Tests only applicable in the case of full hose systems.

~~s~~See also ~~R-117~~OIML R 117-2,- Annexes A and ~~Annex~~ B.

EDR

Annex F

Testing procedures for measuring systems on pipelines and systems for the loading of ships

~~10.1.2~~**F.1** ~~D~~**General i**nformation

The tests in Annex ~~F-D~~ apply to measuring systems used for pipelines and systems for the loading of ships. These procedures are for all liquids with the exception of systems for potable liquids (foaming or non-foaming).

In accordance with ~~Section OIML R 117-1, 2.10.4 of part 1~~, higher viscous liquids are covered by Annex ~~FD~~, but are not required to have gas elimination devices fitted. ~~-~~ In this case, provisions must be made to prevent the entry of air into the system as per section ~~OIML R 117-1, 5.7.2 of part 1~~.

F.1.1 ~~D~~**Type a**pproval

Measuring systems on pipelines and systems for loading of ships (to be referenced as “~~Measuring Systems~~MS” for the remainder of this ~~A~~nnex ~~section~~) consist of several constituent elements ~~which. These constituent elements~~ may or may not be subject to a separate type approval. ~~-~~According to ~~OIML R 117-1, 6.1.1 of part 1~~, the constituent elements of a ~~measuring system~~MS shall comply with the relevant requirements.

The type ~~evaluation~~approval of ~~measuring systems~~MS involves verifying that the constituent elements of the system, which have not been subject to separate type approvals, satisfy the applicable requirements.

Tests for carrying out the type approval of ~~measuring systems~~MS shall therefore be determined on the basis of the type approvals already granted for the constituent elements.

When none of the constituent elements have been subjected to separate type approval testing, the tests provided in ~~sections~~ 5, 6, 7, and 8 shall be performed as required on the applicable elements.

~~On the contrary, when~~When all of the various constituent elements are approved separately, it ~~may~~shall be possible to perform type evaluation of the complete measuring system~~MS the system type approval~~ based on a review of systems drawings and a review of the type approval drawings / certificates of the individual constituent elements.

These types of ~~measuring systems~~MS are usually single-unit productions built for a specific application. ~~-~~To take this fact into account, type approval tests are typically carried out for the individual constituent elements. The testing of the complete ~~measurement system~~MS is normally completed during the initial verification.

In some cases, it may not be possible to test a complete measuring system~~MS where it is (or will be) installed. - in situ, in -~~ In this case, it is possible to test the constituent elements in a test facility having comparable conditions as long as the ~~systems~~hydraulic conditions of the system can be closely replicated. ~~-~~ taking into account the requirements of ~~R 117 R 117~~OIML R 117-2, ~~s~~Section 5.3.4. ~~of part 1~~.

F.2 ~~F.1~~**Metrological controls and performance tests for type** ~~evaluation~~approval

F.2.1 ~~F.1.1~~**Testing procedures for meter sensors, measuring devices and meters with mechanical indicating devices**

Testing is completed in accordance with ~~Section~~ 5. These tests include:

- ~~A~~accuracy tests;

- ~~t~~Tests on the minimum measured quantity; and
- ~~e~~Endurance testing.; and

Notes:

Reverse flow prevention as per ~~OIML R 117-1, section 5.7.3 of part 1~~ (Uni-~~D~~irectional ~~S~~system) and reverse count detection (Uni-~~D~~irectional and ~~B~~bi-~~D~~irectional ~~S~~systems) shall be verified.

A ~~s~~Sampling device (if present) shall be verified as per ~~OIML R 117-1, section 5.7.4 of part 1~~.

F.2.2 Testing procedures for electronic devices: calculator, correction, indicating, and associated devices

Testing is completed in accordance with ~~Section 6~~.

Notes:

The ~~c~~Checking ~~F~~facility shall be ~~of~~ permanent and automatic (Ttype P) and result in a visible or audible alarm for the operator. ~~T~~; this alarm shall continue until the ~~flow-rate~~flowrate and other operating conditions are ~~is~~ within the ~~allowed~~restricted limits.

F.2.3 If the ratio between the maximum and minimum ~~flow-rate~~flowrate of the ~~measuring system~~MS is less than 5, verify that the requirements of ~~OIML R 117-1, section 5.7.1 of part 1~~ are fulfilled.**F.1.3** Testing procedures for gas elimination devices

Testing is completed in accordance with ~~Section 7~~. ~~–If the entry of air into the liquid or release of gas from the liquid is prevented by the configuration of the pipework or by the arrangement and operation of the pump(s), this system arrangement shall be fully documented.~~

Notes: 1) ~~–The s~~System shall meet the requirements of ~~OIML R 117-1, section 5.7.2 “Prevention of gas flow” from part 1~~.

Note 2: 2) If system is not fitted with a gas elimination device, the requirements of ~~OIML R 117-1, Sections 2.10 and 5.1.3 of part 1~~ shall be fulfilled.

Note 3: 3) It is assumed here that ~~section section 7~~ will either include a complete set of testing procedure for larger gas elimination devices, or develop a methodology to derive performance of high capacity devices from that of smaller devices of similar design.

F.2.3 ~~F.1.4~~ Testing procedures for ancillary devices

Testing is completed in accordance with ~~Section 8~~.

Annex G

Testing procedures for measuring systems for the fueling of aircraft

G.1 General information

Most aircraft refuelling tank vehicles and vehicles/carts with hydrant measuring systems are designed for use at airport locations and ~~are not designed~~ for travel on regular roads (because of vehicle size limits, maximum axial load, hanging parts, etc.). Therefore, in most cases, it is necessary to ~~do~~perform the test procedures of Annex G on the site of use at an airport.

Measuring systems intended for the fuelling of aircraft usually consist of several constituent elements which. ~~These constituent elements~~ may or may not be subject to a separate type approval.- According to OIML R 117-1, 6.1.1 ~~of OIML R-117~~R 117-1, the constituent elements of a measuring system shall comply with the relevant requirements.

The type approval of a measuring system intended for the fuelling of aircraft consists of verifying that the constituent elements ~~of the dispenser~~, which have not been subject to separate type approvals, satisfy all applicable requirements.

Tests for carrying out the type approval of a measuring system ~~intended for the fuelling of aircraft~~ shall therefore start with a full review of the type approvals already granted for the constituent elements of the measuring system.

When none of the constituent elements has been subject to separate type approval, all the tests provided in sections 4, 5, 6, and 7 shall be performed. When the various constituent elements have been approved separately, it may be possible to replace type approval based on tests by type approval of drawings of the constituent elements.

Measuring systems for fuelling aircraft are usually single-unit productions (they are not mass-produced). To take this fact into account, the approval tests are usually carried out on the individual components. The testing of the complete measurement system is usually most suitable for initial verification testing.

Before conducting tests, it is necessary to execute the design evaluation of the measuring system ~~intended for fuelling aircraft~~ by using the general check-list given in ~~R-117~~R 117-3 and the relevant points of this Annex G.

G.2 Metrological controls and performance tests for type approval

G.2.1 Testing procedures for meter sensors, measuring devices and meters with mechanical indicating devices

Testing is completed in accordance with ~~(the applicable parts) of Section-5~~. These tests include:

- ~~A~~accuracy tests;
- ~~t~~Tests on the minimum measured quantity;
- ~~e~~Endurance testing; ~~and~~
- ~~n~~Non-return valve configuration and reverse count detection; ~~and~~
- ~~f~~Flow disturbance test (if necessary).

G.2.2 Testing procedures for electronic devices: calculator, correction, indicating, and associated devices

Testing is completed in accordance with ~~Section-6~~.

G.2.3 Testing procedures for gas elimination devices

Testing is completed in accordance with ~~Section~~ 7.

Note: ~~If a M~~measuring systems for the fuelling of aircraft ~~is-are typically~~ not fitted with a gas elimination device. ~~In this case~~, the requirements of OIML R 117-1, Sections 2.10 and 5.1.3 of R117R 117-1 shall be fulfilled.

G.2.4 Testing procedures for ancillary devices

Testing is completed in accordance with ~~Section~~ 8.

G.2.5 Additional test procedures for the complete measuring system intended for the fuelling of aircraft

G.2.5.1. -Common tests for all measuring systems intended for the fuelling of aircraft

Object of the test

To determine the accuracy of the quantity indication of the stationary or mobile measuring system intended for refuelling of aircraft during delivery.

Test procedure

The delivery starts from an appropriate source of delivered liquid (pipeline or tank upstream of the measuring system).

It is necessary to ensure that- the liquid level in the tank remains above its lowest permissible level during testing.

The test quantity shall be at least the volume delivered in one minute at the tested flowrate.

Test procedure using a volumetric test measure:

- 1) Recirculate the system to stabilize the system temperature and pressure. Always stop the delivery by the nozzle or by valve closest to the test measure.
- 2) Wet and drain the test measure.
- 3) Reset the indication of the CID.
- 4) Start the filling procedure of the test measure from the liquid source at the service flowrate (recommended to be in the range of 0.8–1 ~~of~~ Q_{max}).
- 4.5) Read p_t and T_t
- 6) Read V_i , V_s , T_s .
- 7) Calculate V_n and E_{vi} .
- 2.8) Drain the test measure.
- 9) Evaluate, determine if the result is within the MPE.
- 10) If yes, repeat steps 3 to 8, check if those results differ by more than 0.05 %.
- 11) If yes, repeat steps 3 to 8 again.
- 3.12) Then calculate the mean value \bar{E}_v .
- 13) Fill in the test report.

Repeat this test procedure for flowrate (recommended $Q_{\min} = 0.2 \cdot Q_{\max}$) and for intermediate Q .- Intermediate Q should be a point where meter is expected to be least accurate.

Repeat this test procedure for the MMQ.

The ~~m~~Mean values of ~~the~~ error of the tested flowrates -shall not exceed ± 0.2 %.

Repeatability shall not exceed 0.05 %.

Test procedure using a ~~M~~master ~~M~~meter:

- 1) Recirculate to stabilize ~~the~~ system temperature and pressure. Always stop the delivery by the first valve downstream of ~~m~~Master ~~M~~meter.
- 2) Reset the indication of the ~~M~~master ~~M~~meter.
- 3) Reset the indication of the CID.
- 4) Start the filling procedure from the liquid source at ~~the~~ service flowrate (recommended about $0.8 \cdot Q_{\max}$).
- 5) Read $-V_n$ and calculate E_{vi} .
- 6) Evaluate, determine if the result is within the MPE.
- 7) If yes, repeat steps 2 to 8, check if those results differ by more than 0.05 %.
- 8) If yes, repeat steps 2 to 8 once more.
- 9) Then calculate the mean value \bar{E}_v .
- 10) Fill in ~~the~~ test report.
- 11) Repeat this test procedure for flowrate (recommended $Q_{\min} = 0.2 \cdot Q_{\max}$) and for the intermediate flowrate. -The intermediate flowrate should be a point where the meter performance is the worst.

Repeat this test procedure for the MMQ if it is smaller than 500 L.

The ~~m~~Mean values of ~~the~~ error between tested flowrates shall not exceed ± 0.2 %.

Repeatability shall not exceed 0.05 %.

Note: -It is also possible to fulfill the requirements of this section gravimetrically.

Annex X

Interpretation, ~~eE~~Examples, ~~Aa~~Advice, and ~~Pp~~ossible ~~Ss~~olutions

X.2 Chapter 2

The figure below is added in Annex X to assist with the understanding of constituent elements of a measuring system. ~~T~~~~(~~the blue double line represents the liquid flow; the flow control system consists of the pumps, valves, etc.~~)~~.

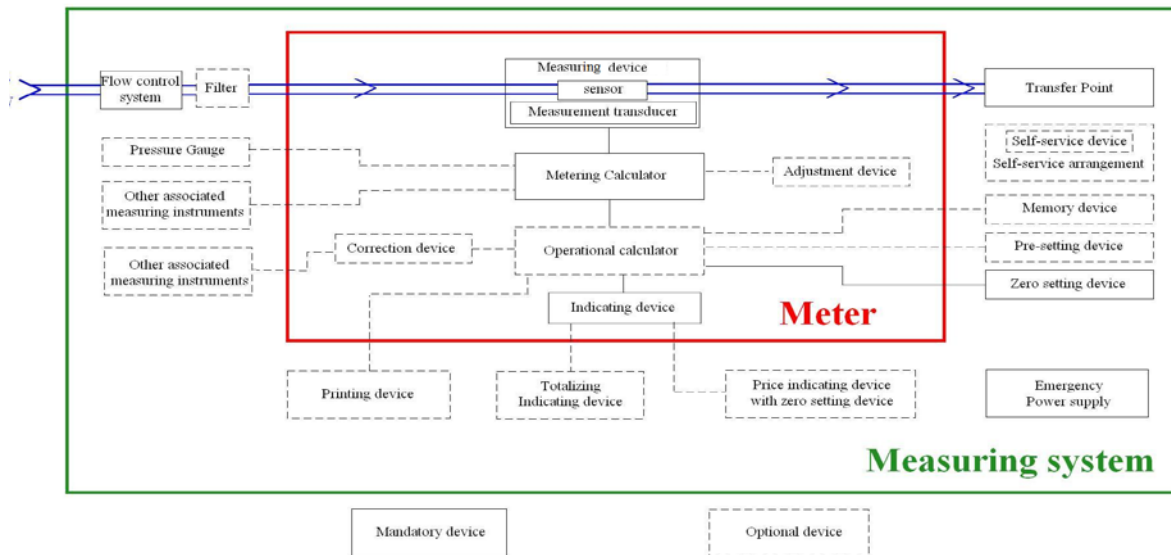


Table X.2.1

-Section from R 117 OIML R 117-1	General metrological requirements for <u>specific components</u> of a measuring system																		
	Meter						Gas elimination device			Associated measuring devices			Ancillary device (main examples)						
	Measuring device				Electronic calculator	(incl. conversion, adjustment, compensation)	Indicating device	Gas separator	Gas extractor	Special gas extractor	Pressure measuring device	Density measuring device	Temperature measuring device	Self-service device	Printing device	Memory device	Price indication device	Pre-setting device	Conversion device (not included in calculator)
	Meter sensor		Transducer																
	Electrical	Mechanical	Electrical	Mechanical															
1.2	X	X																	
2.2														X	X	X	X	X	X
2.5	X	X	X	X	X	X													
2.6.2	X	X	X	X	X	X					X	X	X						
2.6.3	X	X	X	X	X	X													
2.7.1					X						X	X	X						X
2.7.2					X						X	X	X						X
2.8					X														
2.9.1						X					X	X	X						
2.9.2						X													X
2.10.1							X	X	X										
2.10.2							X	X	X										
2.10.3							X	X	X										
2.10.5							X	X	X										
2.10.7							X	X	X										

-Section from R117R-117OIML R 117-1	General metrological requirements for <u>specific components</u> of a measuring system																	
	Meter						Gas elimination device			Associated measuring devices			Ancillary device (main examples)					
	Measuring device				Electronic calculator (incl. conversion, adjustment, communication)	Indicating device	Gas separator	Gas extractor	Special gas extractor	Pressure measuring device	Density measuring device	Temperature -measuring device	Self-service device	Printing device	Memory device	Price indication device	Pre-setting device	Conversion device (not included in calculator)
	Meter sensor		Transducer															
	eElectrical	mMechanical	eElectrical	mMechanical														
2.10.8						X												
2.10.9								X	X									
2.19.2	X	X	X	X	X	X	X	X	X	X	X	X	X	X	X	X	X	X
2.19.4						X												
2.20.1	X	X	X	X	X	X	X	X	X	X	X	X	X	X	X	X	X	X
2.20.2					X	X							X		X			X
3.1.1	X	X	X	X	X	X												
3.1.2	X	X	X	X	X	X												
3.1.3			X	X	X													
3.1.4			X		X					X	X	X						
3.1.5		X	X	X	X	X												
3.1.6	X		X		X	X												
3.1.7	X		X		X	X												
3.1.8	X		X		X	X												
3.1.9	X		X		X	X												
3.1.1																		

-Section from R117R-117OIML R 117-1	General metrological requirements for <u>specific components</u> of a measuring system																
	Meter					Gas elimination device			Associated measuring devices			Ancillary device (main examples)					
	Measuring device				Indicating device	Gas separator	Gas extractor	Special gas extractor	Pressure measuring device	Density measuring device	Temperature -measuring device	Self-service device	Printing device	Memory device	Price indication device	Pre-setting device	Conversion device (not included in calculator)
	Meter sensor		Transducer														
	eElectrical	mMechanical	eElectrical	mMechanical													
3.2					X												
3.3															X		
3.4													X				
3.5														X			
3.6																X	
3.7																	X
3.8					X												
4.1	X		X		X	X											
4.2					X	X											
4.3.1	X		X		X	X							X				X
4.3.2	X		X														
4.3.3					X							X		X??			
4.3.4						X											
4.3.5												X	X	X	X	X	X
4.3.6									X	X	X						

X.10X.5 Chapter 5 (Testing procedures for meter sensors and measuring devices)

X.5.1 If the meter sensor/measuring device is tested in a complete fuel dispenser (especially at lower flowrates), a temperature rise during the successive tests can occur. To avoid such a temperature rise, a connection with a non-return valve and flow regulating valve from the pipe between the gas separator and the meter sensor, measuring device or meter to the supply tank can be installed. At lower flowrates, the main liquid flow is fed back to the storage tank via this extra outlet.†

Every time the meter sensor/measuring device to be tested is connected hydraulically, it should be operated at the maximum flowrate for at least five minutes (e.g. to reach stability of [liquid] temperature and removal of air/gas) before measurement starts. ~~Every time a new work session starts (for example after a stop of one hour or more), the EUT should operate at the maximum flowrate for at least one minute or until metrological stability is achieved, before the measurement starts.~~

X-5.3.3 Advice on Section 5.3.3 (continued)

Testing at the limits of the rated operating conditions may not be required when these limits have a negligible effect on the specific meter technology. (For example, it would not be necessary to test a mass flow meter at the limits of viscosity, or a meter with a pressure-balanced measuring chamber at the limits of pressure).

When it is determined that the rated operating conditions will affect the accuracy of the meter, the following may be considered:

- tests at the limits of pressure are not needed if the maximum liquid pressure is equal to or below 10 bar;
- tests at the limits of pressure may be conducted within ± 10 bar of the actual limit;
- tests on a liquid with a viscosity up to 1 mPa·s may be used to represent liquids with viscosities up to 2 mPa·s;
- tests at the limits of viscosity > 2 mPa·s may be within ± 20 % of the actual limits;
- tests at the limits of liquid density may be within ± 100 kg/m³ of the actual limits.

Where the measuring system is intended to measure liquid quantities at temperatures from -5 °C to $+35$ °C, only one accuracy test at one temperature between -5 °C and $+35$ °C is suggested.

X.5.3.4 Advice on ~~F~~flow disturbance ~~Section 5.3.4~~

A few disturbance configurations are provided in the case that flow disturbance testing is performed:

- two elbows ~~out of in the same~~ plane upstream of the meter or the measurement transducer;
- ~~two elbows in the same plane upstream of the meter or the measurement transducer; and two elbows in the same plane upstream of the meter or the measurement transducer;~~
- a locked propeller upstream of the meter or the measurement transducer;
- a locked propeller downstream of the meter or the measurement transducer;
- a valve upstream of the meter or the measurement transducer in several positions (90° , 80° , 65° , 45°).

If necessary, additional disturbance configurations may be defined by the technology of the meter.

X.5.4 Determination of the flowrate

The flowrate can be obtained under flying start/stop conditions by the following procedure:

Start the flow. When the indication is at a whole number of litres/kg (V1), start the stop-watch.

After at least 30 seconds, stop the stop-watch when the indication is at a whole number of litres or kilograms (V2).

Calculate the flowrate $Q = (V2 - V1) \times (60 / t)$ in L or kg/min

(Where: t = the time elapsed in seconds, from the stop-watch in step 3).

~~*unless outside the prescribed range (normal use)~~

~~## external vibration in use~~

~~Temporary Convenor Note 1: The project group spent a very significant amount of developing, discussing, editing, and arguing about this "Table showing whether different meter technologies are affected by various operating conditions." The participants at the Teddington meeting (Oct 2013) decided that it was best to not include the table in the 2CD because consensus on its contents could not be reached. The convenor continues to believe that the table would have value if consensus could be reached ... so, it has been left (in lineout form) to encourage Project Group members to comment on whether the table should be included and the table's suggested practices~~
X.5.4.3
 (continued) — Testing at the limits of the rated operating conditions may not be required when these limits have a negligible effect on the specific meter technology. (For example, it would not be necessary to test a

~~mass flow meter at the limits of viscosity, or a meter with a pressure balanced measuring chamber at the limits of pressure).~~

~~When it is determined that the rated operating conditions will affect the accuracy of the meter, the following may be considered:~~

- ~~• tests at the limits of pressure are not needed if the maximum liquid pressure is equal to or below 10 bar;~~
- ~~• tests at the limits of pressure may be conducted within ± 10 bar of the actual limit;~~
- ~~• tests on a liquid with a viscosity up to 1 mPa·s may be used to represent liquids with viscosities up to 2 mPa·s;~~
- ~~• tests at the limits of viscosity > 2 mPa·s may be within ± 20 % of the actual limits; • tests at the limits of liquid density may be within ± 100 kg/m³ of the actual limits.~~

~~Where the measuring system is intended to measure liquid quantities at temperatures from -5 °C to $+35$ °C, only one accuracy test at one temperature between -5 °C and $+35$ °C is suggested.~~
X.5.6 XAdvice on Section 5.6 5.7

Advice/remarks:

~~Please Note~~ that plain water will freeze during a test on low temperatures, in which case the EUT ~~would~~ no longer operate normally.

To prevent damage to the flowsensor due to temperature expansion or contraction, do not close the sensor by means of rigid blinding flanges.

Also keep in mind that in some liquids, bubbles will appear for example by dissolving air. Especially when testing ultrasonic flowmeters, this could cause ultrasonic signals to be interrupted, which is an undesired effect.

Before the temperature of the liquid is fully stabilized, temperature convection will cause small flows of liquid to move up and down through the EUT. On some meters this will appear as a flow indication where none is expected.

Advice on 5.6 Test ~~m~~Method ~~I~~influence test type A

Calculation example:

Flowrate under reference conditions: 0.0400 L/min

Flowrate under test conditions: 0.0500 L/min

Flow range to be tested: 5—100 L/min

Change in flowrate: $0.05 - 0.04 = 0.01$ L/min

$(0.01 / 5) \times 100 \% < 0.3 \%$

$0.2 \% < 0.3 \% \rightarrow \text{OK}$

Precautions for EUT's with installation dependent characteristics:

Some measurement characteristics may to some degree be affected by the way an electronic meter is installed in a system (the zero-setting of a Coriolis meter for example).

When this is the case, care must be taken that the EUT is not moved nor its installation changed between the reference test and the other tests.

Ambient temperature tests for ultrasonic flowmeters:

Possibly, ultrasonic flowmeters are fitted with an internal temperature transmitter to perform corrections for changes in the meter body's dimensions due to temperature expansion—/—contraction. Based on information provided by the manufacturer and/or knowledge of physics, it should be checked by calculation which part of the observed changes can be ~~attributed~~ attributed to changes in the dimensions of the EUT and which is caused by effects on the EUT's electronics for which these tests are intended.

Ambient temperature tests for electromagnetic flowmeters:

If equipped with a temperature transmitter for corrections, the same applies as for the ultrasonic flowmeters.

Ambient temperature tests for Coriolis meters:

Most Coriolis meters are equipped with an internal temperature transmitter for the purpose of correction. Due to changing measurement tube temperature, the EUT's characteristics will change during the ambient temperature tests. To test the effects on the EUT's electronics separately, this mechanical effect can be eliminated. When one pick-off coil is connected in parallel to both applicable inputs, the mechanical effect of temperature changes is eliminated.

Advice on 5.6 ~~5.7~~ Test ~~m~~Method ~~i~~nfluence test type B

For precautions, see ~~i~~nfluence tests type A.

X 5 Advice ~~to on~~ Chapter 5 concerning meter types:

Low-~~F~~low-~~C~~ut-off

Possibly in electronic meters a so-called low-flow-cut-off is installed. This feature will consider flowrates below this value not to be a measurement. Once a flowrate higher than this value is registered, will the flowrate (without subtraction of the low-flow-cut-off value) be registered as a measurement. During testing, in most cases, it is desirable to see all flow indications, even if below the normal low-flow-cut-off value. Therefore, during most performance tests the low-flow-cut-off should be set to zero.

~~Please Note~~ that in practice an indication other than zero is needed during testing. Generally, the value in practice depends on the zero-stability of the meter, the minimum measured quantity of the complete measuring instrument/-system and the application itself.

Meter curve, electromagnetic flowmeters

Meter performance of an electromagnetic flowmeter is typically determined by the electric conductivity of the liquid and the flow profile.

Meter curve, ultrasonic flowmeters

Several effects determine the metrological behaviour of ultrasonic flowmeters:

The acoustic damping of the liquid:

If the amplitude of the signal decreases to much, the signal to noise ratio becomes so small that the measurement signal becomes unreliable.

The flow profile of the liquid through the measurement sensor:

From the speed of the liquid through the measurement paths, the average flowrate is determined. This is done by applying a weighing factor to the liquid speeds measured through particular paths. If these do not represent the actual flow profile, an incorrect flowrate is determined.

The Reynolds number:

Basically an ultrasonic flowmeter is a Reynolds dependent device. The combination of the sensor's inner diameter, the average speed of the liquid, the liquid density and the liquid viscosity determine the Reynolds number. Therefore the operating range of an ultrasonic meter can be given as the ranges of each of these factors or as a Reynolds range.

Gas bubbles and solid particles:

Both gas bubbles and solid particles contained within the liquid affect the meter's performance due to the fact that they disturb/reflect the ultrasonic signal. Moreover, if the signal is not disrupted, the volume of gas bubbles will be attributed to the liquid volume. However, when the signal is disrupted by gas bubbles or solid

particles, this can be detected by an ultrasonic meter. Detection of such events can be followed by a correcting action, such as for example stopping the flow. If the flow is interrupted quickly enough, the effect of gas bubbles and/or solid particles can be reduced to acceptable proportions. The sensitivity of an ultrasonic meter to gas bubbles and/or solid particles will depend on many factors. Therefore, specific tests would need to be done to prove that the effects are within acceptable limits.

Meter curve, Coriolis meters

Typically, liquid density and/or liquid pressure may have an effect on the device's metrological characteristics. Possibly, effects are automatically corrected for, but in some cases the meter curve may need to be determined under pressures and/or on liquids of a similar density and/or pressure as present in the end-application.

If it is proved ~~in~~ during a type approval, that the effects given-listed above are negligible or properly corrected for, a Coriolis meter's curve can be determined on a liquid which is not similar to the one in the end-application. In that case a meter curve determined on water could for example suit an application on LPG.

Installation effects on Coriolis meters:

The meter's installation dependent ~~zero-setting~~zero-setting affects the metrological behaviour of the device. Therefore, it must be checked that the ~~zero-setting~~zero-setting is correct, once the device is installed. The documentation, manuals, ~~and~~ type approval certificate must state when ~~zero-setting~~ must be performed (for example when the installation has been disturbed, change of liquid, change of temperature).

Coriolis sensor:

All Coriolis meters basically consist ~~out~~ of two sensors: one flowsensor (usually consisting ~~out~~ of one or two parallel measurement tubes) and a temperature sensor for the ~~benefit-purpose~~ of performing temperature corrections on the vibrational properties of the flowsensor.

The primary measurement signals of a Coriolis meter are the following:

- a time difference related to the mass flowrate through the flowsensor;
- a resonant frequency related to the density of the liquid in the flowsensor;
- a resistance related to the temperature of the measurement tube(s).

The measurement tube(s) is/are set into motion (a sinusoidal vibration) by means of an alternating current through one or more so-called drive coils. The movement of the measurement tubes is detected using at least two pick-off coils. In principle these coils are considered to be electronic components, thus making a Coriolis flowsensor an electronic device, on which the applicable performance tests need to be performed. However, the measurement tubes themselves are purely mechanical components. Only when it is proved ~~in~~ that these coils are sufficiently insensitive to the effects of the test conditions, is it allowed not to submit the Coriolis flowsensor to influence/disturbance tests.

Density measurement:

In principle all Coriolis meters perform both a mass flowrate and a density measurement. Both the mass and/or the volume of liquid can be the bases for the measurement transaction. If so desired by the applicant, both the mass and volume output of the equipment under test can be tested against legal requirements. In the case of a Coriolis meter, volume is calculated from measured mass and measured density. So once it is determined that the calculation of volume operates correctly, verification of the mass and density determination suffices to guarantee the correctness of the Coriolis meter's mass and volume outputs.

Effect of liquid properties:

Some Coriolis meters may be affected by the density of the measurand, in which case the meter curve will shift dependent of the liquid density.

Extremely high liquid viscosities ~~also~~ may also have an effect. This is thought to be caused by the liquid absorbing the vibrational energy of the measurement tubes, thus reducing the amplitude of the vibration. In


extreme cases such a reduction will cause the measurement signals to become too small for correct processing. Such effects occur especially when the flow is started.

FEDOR

X.7 Advice Annex for Section 7 “Test procedures for gas elimination devices”

X.7.4 Figure 1 – Test bench for gas separators

(Also:- Test bench for gas separators in fuel dispensers)

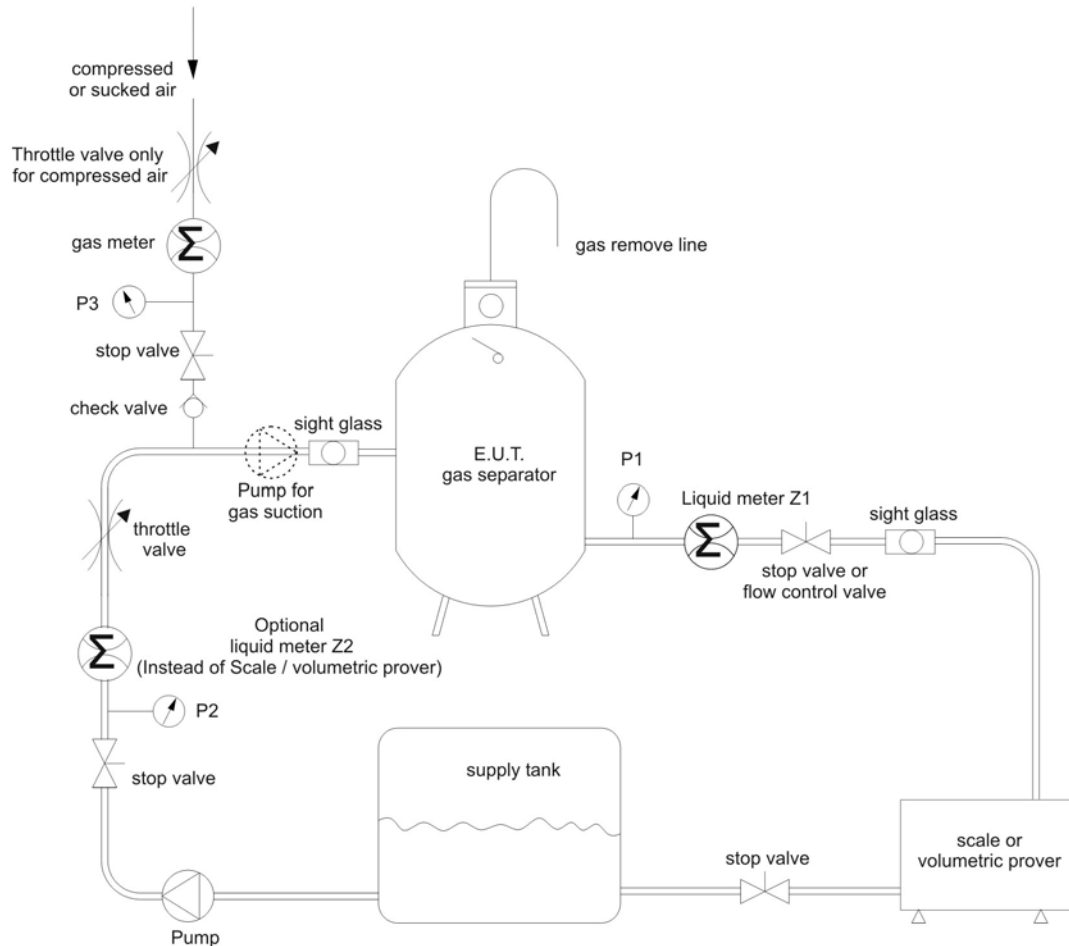

Gas is introduced into the test liquid when the valves in the gas supply line are open. The gas flow is set by the throttle valve and the gas meter. By manometer P3 the actual gas volume is converted to atmospheric pressure.

Two optional test methods:


- The liquid volume $V_{n-(\text{without gas})}$ of the delivered liquid is measured by the scale/-volumetric prover and the volume V_i delivered over the gas separator is measured by the liquid meter Z1.
- The liquid volume $V_{n-(\text{without gas})}$ is measured by the liquid meter Z2 and the volume V_i delivered over the gas separator is measured by the liquid meter Z1.

The precondition for this test is that before and after the test the gas separator is completely filled resp. filled to the same extent.

X.7.4 Figure 2 – Test bench for gas extractors (gas pocket test)

Also: Air pocket test bench for refinery applications

~~The~~the volumetric prover could also be a gravimetric scale.)

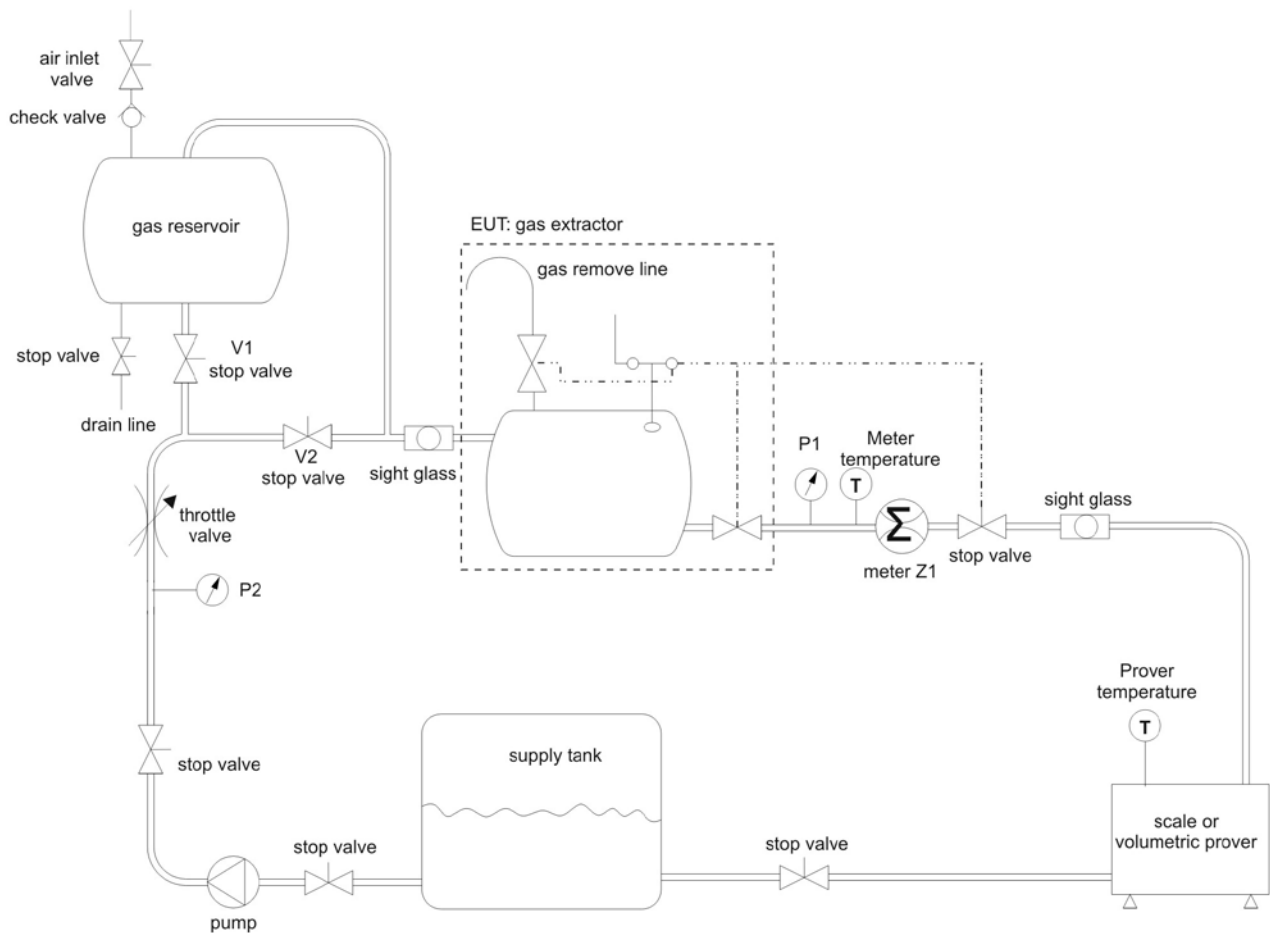


The gas pocket is created in the gas reservoir with stop-valve V1 kept closed. The required volume of the gas pocket is created by filling up the gas reservoir with liquid to the known volume of the gas reservoir and then by draining it partially over its drain valve.

For the test run the gas pocket is discharged from the gas reservoir to the liquid stream by opening valve V1 completely and closing valve V2.

X.7.4 Figure 3 – Test bench for special gas extractors

+



No.:	Component	Name
1	Storage tank	B2, B1
2	Test container	B3
3	Foot valve	V2, V1
4	In-line valve	V4, V3
5	Stop valve	V5, V6, V21, V16
6	Ball valve	V17
7	Check valve	V15
8	Throttle valve with sight glass	V23
9	In-line valve	V24, V26, V27
10	Throttle valve	V34
11	Sight glass	S1, S2, S3, S4
12	Pressure manometer	P1, P3
13	Thermometer	T2, T1
14	Pump	K1, K2
15	Scale	W1
16	Positive displacement meter	Z1
17	High pressure gas meter	Z2
18	Rotameter	Z3

X.7.4, Table 1: System components of the test bench

- Heights h_1 and h_2 :

For gravity discharge tests a static height difference (h_1) between the supply tank and the meter and a static height difference (h_2) between the meter and the tank on the scale (B3) shall be provided. Height h_1 shall be at least above the level where the special gas extractor and meter are completely filled. By opening the valves of the supply tanks the special gas extractor is completely flooded. Before testing, the pipework from the supply tanks up to the automatic stop valve (V21) is completely filled with liquid. For a high ~~flow~~ ~~rate~~ flowrate height h_2 should be as large as possible.

The use of a suction pump at the outlet of valve (V23) is not recommended, because determining the start and end conditions of remaining product in the pump is not well defined.

- Pipe connection for pumped and gravity discharge tests:

During gravity discharge tests valve (V5) is open. The test liquid flows via the bottom valve (V1 and/or V2), (V5) and (V6) to the special gas extractor. The ~~flow~~ ~~rate~~ flowrate is throttled via the valve (V23) to make sure that meter (Z1) is constantly flooded. Make sure that the liquid pressure directly downstream of the meter is not below atmospheric pressure.

For pumped discharge tests valve (V5) has to be closed and the pump K1 has to be switched on.

- Residual discharge test of the gas extractor function:

The delivery of liquid is carried out either from supply tank (B1) or (B2). The pipe route is enabled depending on the type of test (gravity discharge or pump operation).

The throttle valve (V23) is fully open. After the start of the delivery the stop valve (V21) is opened and the liquid flows through the special gas extractor into the tank on the scale (B3). In the case of gravity discharge, the throttle valve (V23) has to be set such that the liquid pressure at manometer P3 is never below the atmospheric pressure.

After each test run the liquid pipework from the bottom valve of the supply tank in use to the discharge pipe (V21) is ventilated.

- Empty compartment test of the gas extractor function:

The delivery of liquid is carried out by filling one of the two supply tanks with test liquid whereas the other supply tank is completely empty. The valves in the pipes are switched depending on the type of test (gravity discharge or pump operation). After the start of the delivery the automatic stop valve (V21) opens and the test liquid flows through the special gas extractor into the weighing tank (B3).

During the delivery the liquid path is switched from the supply tank in use to the empty supply tank. When the special gas extractor comes into action the liquid path is switched back to the supply tank. After each test run, the liquid pipework from the bottom valves of the supply tanks to the discharge pipe (V21) is ventilated.

- Test of the gas separator function with continuous gas supply:

A continuous supply of gas is added to the liquid by opening valve (V17). The gas flow is set by a throttle valve (V34), a gas meter (Z2) and a gas ~~flow~~ ~~rate~~ flowrate sensor (Z3).

Valve (V16) will be automatically opened, when the automatic stop valve (V21) is released by the special gas extractor and liquid is flowing.

The delivery of liquid is carried out by filling the supply tank (B1) or (B2) with liquid. The valves in the pipes are switched depending on the type of test (gravity discharge or pump operation). After the start of the delivery the automatic stop valve (V21) is opened. The liquid flows through the special gas extractor into the tank on the scale (B3).

During the delivery, a continuous flow of compressed gas is simultaneously introduced into the liquid pipework. When the liquid measuring process is interrupted by the special gas extractor, the automatic stop

valve (V21) and the valve (V16) are closed and the flow of the liquid and compressed gas supply is interrupted.

By the gas meter (Z2) and the manometer (P2), the percentage of gas volume related to the liquid volume can be calculated.

After each test run the liquid pipework from the bottom valves to the discharge pipe (V21) is ventilated.

FOR

Annex X.A (non-mandatory)

This part of Annex X contains “Advice and ~~S~~suggested ~~P~~practices” concerning:

- Testing procedures for fuel dispensers (type evaluation advice and suggested practices) – these Sections are numbered X.A.n.n.n and correspond to the Sections numbered A.n.n.n in Annex A;
- Draft testing procedures for fuel dispensers (for initial verification) – these Sections are numbered X.A-I.n.n.n and start in Section X.A-I.7.
- Testing procedures for LPG dispensers (type evaluation advice and suggested practices) – these Sections are numbered X.A-LPG.n.n.n and correspond to the Sections numbered A.n.n.n in Annex A;
- Draft testing procedures for LPG dispensers (for initial verification) – these Sections are numbered X.A-LPG-I.n.n.n and start in Section X.A-LPG-I.nn.

~~Note: — a decision to not include the initial verification test procedures in the (mandatory) Annexes of the 2CD of R117R-117-2 was made at a Project Group meeting in Teddington in October 2013. Instead, these draft initial verification test procedures are planned to be part of the next revision cycle of R117R-117.~~

X.A.2.1 Accuracy tests

- ~~2)a)~~ Determine Q_{\min} and Q_{\max} for the associated viscosity/defined fluid to be measured.
- ~~3)b)~~ Put the meter on the test rig as per the manufacturer's specifications, see ~~OIML R117R-117OIML R 117-2, section 5.1.~~ The test rig might include a pump, associated piping, feeding tank, control valves, hose and nozzle. None of these parts shall interfere with the performance of the meter under test. If the test rig is provided by the manufacturer, it shall be capable of ensuring that no air or vapor is fed to the meter during testing (no cavitations).
- ~~4)c)~~ Adjust the meter to the closest ~~zero setting~~zero-setting at the highest applicable ~~flow rate~~flowrate for approval (or at least 80 % of such a value as per the requirement of the manufacturer).
- ~~5)d)~~ If more than one adjustment point is needed, refer to the manufacturer's adjustment procedure (i.e. in the case of a multipoint adjustment curve for dynamic adjustment).
- ~~6)e)~~ Secure the adjustment setting as it shall remain unchanged for X.A.2.1.g, X.A.2.2 and X.A.2.3. ~~-Any change to the adjustment settings of the meter before the end of the tests related to sSection A.2.3 will invalidate the test results related to sSections X.A.2.1.g, X.A.2.2 and X.A.2.3. Securing the adjustment setting shall be achieved with adequate seals or isolation of the EUT in a room/building until the tests related to sSection X.A.2.3 are finished.~~
- ~~7)f)~~ Establish the list of flowrates to be tested as per ~~OIML R117R-117OIML R 117-2, section 5.3.2.1.~~
- ~~8)g)~~ Carry out testing for each flowrate (see 5.3.2.1) and record the accuracy test results. All results shall be within the applicable MPE.
- ~~9)h)~~ Repeat g) at the limits of operation as per ~~OIML R117R-117OIML R 117-2, clause 5.3.3.~~
- ~~10)i)~~ If applicable, repeat g) with different disturbances as per ~~OIML R117R-117OIML R 117-2, clause 5.3.4.~~

X.A.2.2 Tests on the MMQ (with maximum specified hose length if applicable)÷

- ~~a)~~ Confirm adequate hose arrangement for type approval – Flush hose with 3 minutes of continuous flow to remove any remaining air bubbles.
- ~~b)~~ Activate the pumping system to pressurize the instrument/meter.
- ~~c)~~ Stop the pump – leave idle for 1 minute.

- ~~d~~) Reset ~~the~~ indication, activate ~~the~~ pump, pressurize ~~the~~ instrument/meter and deliver a quantity equal to MMQ at maximum achievable ~~flow rate~~flowrate in the measuring standard.
- ~~e~~) Record ~~the~~ accuracy test result. ~~The r~~Result shall be within ~~the~~ applicable MPE for MMQ as per ~~clause OIML R 117-1, 2.5.32.5.1 of OIML R-117~~R-117-1.
- ~~f~~) Repeat steps b) to e) two more times.

X.A.2.3 Endurance testing - see ~~OIML R-117~~OIML R 117-2, ~~section~~ 5.4

~~The e~~Endurance test and related accuracy tests shall be conducted with a fluid having a low viscosity / low lubrication capacity in ~~the~~ viscosity range requested by ~~the~~ manufacturer.

X.A.2.4 Check of reverse flow prevention

During meter testing, systems which are designed to cope with reverse flow shall be assessed, and recorded in ~~the~~ type approval file (description of solution, e.g.: combination of non-return valve and/or reverse pulse counting)

~~The m~~Manufacturer shall provide ~~a~~ test method to demonstrate that ~~the~~ design copes with reverse flow. ~~The~~ test shall be conducted and ~~the~~ result recorded.

Note on ~~OIML R-117~~OIML R 117-1, 2.13.4:

“2.13.4 When reversal of the flow could result in errors greater than the minimum specified

quantity deviation, a measuring system (in which the liquid could flow in the opposite direction

when the pump is stopped) shall be provided with a non-return valve. If necessary, the system shall also be fitted with a pressure limiting device”

It is the purpose of this clause of ~~R-117~~OIML R 117-1 to make sure that reversal flow cannot influence ~~the~~ next transaction when ~~the~~ system ~~get becomes~~ repressurized. Achieving such function with a non-return valve. But such ~~a~~ system requires a pressure limiting device to avoid ~~the~~ hose or piping ~~to bursting~~ open in ~~the~~ case of heat overpressure on ~~the~~ hose (sun radiation) or hose overrun. ~~A M~~modern solution can also imply reverse pulse counting during idle ~~system~~ time ~~of system~~, so repressurizing does not result in errors greater than the minimum specified quantity deviation.

X.A.4 Testing procedures for gas elimination

Requirements on MPE for gas elimination are ~~given~~ in ~~OIML R-117~~OIML R 117-1, ~~section~~ 2.10.1.

Note 1: ~~A~~adequate means shall be used to prevent de-priming the suction line connecting ~~the~~ EUT to ~~the~~ storage tank. ~~An~~ air injection point shall be implemented between such means and ~~the~~ EUT.:

Note 2: A “setting run” ~~can may~~ be needed to set ~~the~~ air intake/~~flow rate~~flowrate to ~~the~~ next Q_i rate before performing ~~the~~ real accuracy test. As ~~the~~ test shall ~~commence begin~~ and stop with ~~the~~ air intake closed (at ~~the~~ end of ~~the~~ accuracy test flow, accurate termination ~~is done achieved~~ with ~~the~~ nozzle trigger), ~~the~~ valve controlling ~~the~~ air intake might be secured with a second valve in-line to stop/start ~~the~~ air-intake without touching ~~the~~ setting of ~~the~~ main air-intake valve.

X.A.6.4.6 ———Temperature conversion (if applicable)

X.A.6.4.6.1 Method 1: use of a measuring standard capable of correcting also for temperature at final reading (as resulting temperature in a readable information with some measuring standards such as proving cans, with probe sensing fuel temperature in the middle if the volume of fuel)

- a) Definition of MPEC (Maximum permissible error with ~~conversion~~~~correction~~). MPEC is the addition of applicable line A or B of ~~Table 2 of OIML R 117-1~~ and ~~line C of OIML R 117-1, Table 2, line C~~ for the applicable class (example: if ~~the~~ EUT is ~~a~~ full measuring system under class 0.5, MPE is 0.5% (line A) and conversion extra MPE is 0.2% (line C) as per ~~OIML R 117-1, clause 2.7.1.2~~).
- b) Use two storage tanks of the same fuel, each at a different temperature. Tank 1 shall be cold, tank 2 shall be warm. ~~The~~ temperature difference between tank 1 and tank 2 shall be at least 10 °C. ~~The~~ length of ~~the~~ connection piping from ~~the~~ tanks to the EUT shall be minimal.
- c) Pre-condition measuring standard on tank 1. Adjust ~~the~~ meter to closest to ~~zero-setting~~~~zero-setting~~.
- d) Execute accuracy test on tank 1. ~~The v~~Volume of ~~the~~ test shall be at least ~~2 × MMQ~~ + volume of piping and no more than ~~4 × MMQ~~ + volume of piping from tank to EUT. Record ~~the~~ result. ~~The r~~Result shall be within ~~the~~ MPEC.
- e) Switch ~~the~~ EUT to tank 2. Do not flow liquid from tank 2 unless it is for the next accuracy test.
- f) Execute ~~the~~ accuracy test on tank 2. ~~The v~~Volume of ~~the~~ test shall be at least ~~2 × MMQ~~ + volume of piping and no more than ~~4 × MMQ~~ + volume of piping from ~~the~~ tank to ~~the~~ EUT. Record ~~the~~ result. ~~The r~~Result shall be within ~~the~~ MPEC.
- g) Switch ~~the~~ EUT to tank 1. Do not flow liquid from tank 2 unless it is for the next accuracy test.
- h) Execute ~~the~~ accuracy test on tank 1. ~~The v~~Volume of ~~the~~ test shall be at least ~~2 × MMQ~~ + volume of piping and no more than ~~4 × MMQ~~ + volume of piping from ~~the~~ tank to ~~the~~ EUT. Record ~~the~~ result. ~~The r~~Result shall be within ~~the~~ MPEC.
- i) When applicable, check ~~the~~ correction table of ~~the~~ calculator (or checksum signature when applicable) and record.

Note 1: The purpose of this ~~m~~Method 1 process is to check ~~the~~ global response of ~~the~~ ~~t~~Temperature conversion, using measurement standards capable of correcting ~~the~~ result with ~~the~~ final temperature of ~~the~~ transferred fuel. As ~~it might not be easy to deploy~~ these means ~~might not be easy to deploy~~ for testing, method 2 allows for split verification for type approval purposes.

Note 2: Special safety precautions shall be in use to prevent ~~any~~ fuel hazard when heating.

X.A.6.4.6.2 Method 2: split EUT verification for type approval

These tests can be ~~done~~~~performed~~ with a low hazard fuel such as mineral spirit.

- a) It is recommended to execute these tests with a low hazard fuel such as mineral spirit.
- b) ~~The~~ EUT arrangement shall be with ~~a~~ very short hose.
- c) Install ~~the~~ reference probe (1) at ~~the~~ EUT temperature well.
- d) Install ~~the~~ reference probe (2) at ~~the~~ EUT nozzle spout tip.
- e) Disengage ~~the~~ temperature correction of ~~the~~ EUT

Note: ———Refer to ~~the~~ manufacturer's manual as this might be the way to have maintenance information displayed on ~~the~~ EUT dial such as ~~the~~ temperature of ~~the~~ fuel at ~~the~~ EUT conversion probe.

- f) Run ~~the~~ flow through ~~the~~ EUT at Q_{\max} from ~~the~~ storage tank for at least 3 minutes to stabilize ~~the~~ fluid temperature and ~~the~~ EUT temperature (outgoing flow can be re-circulated back to storage tank).
- g) Check ~~the~~ accurate temperature reading by comparing ~~the~~ temperature indicated by ~~the~~ EUT (converted signal from its own temperature probe) with ~~the~~ ~~reference~~-reference probe (1) inserted in ~~the~~ temperature well close to ~~the~~ instrument meter/transducer. Maximum difference allowed is 1.6 °C

(equivalent to the 0.2% ~~—line C of OIML R 117-1, Table 2, line C of Table 2 of OIML R-117-1~~ for gasoline).

- h) Warm up the storage tank by 10 °C minimum from the actual temperature.
- i) Read read Probe (1) = PT0, and the temperature indicated by EUT =PTS.
- j) Initiate the flow at Q_{\max} and start the stopwatch simultaneously.
- k) After 15 s (+/- 1 second), read Probe (1) = PT1, probe (2)=PT2 and the temperature indicated by EUT =PTI.
- l) Stop the flow.
- m) If the difference between PT2 and PT1 is greater than 1 °C, ~~redo~~ perform test again or re-assess the test situation.
- n) (PTS-PTI) shall be greater than 90 % of (PT1—PT0).

Note: ~~†~~Testing of g) and k) can be arranged outside of the EUT by using a reference bath to compare the EUT probe reading and the reference probe reading. Such an arrangement also allows for the full range of temperature to be covered.

X.A-I.7 General information for initial verification – Preamble

Initial verification of fuel dispensers may be ~~done~~ performed either:

- a) ~~A~~at the factory of the manufacturer, under quality insurance control, if permitted by the national authority of the country of use;
- a-b) ~~B~~by inspection of the apparatus, routine or batch sample, as per the regulations of the country of use; this is ~~done~~ carried out by the authorized inspection organization;
- c) ~~A~~at the site of use. Common practice is for national authorities to perform this, unless it is subcontracted to an approved/authorized representative of the manufacturer or authority.

Note: -The expression “measuring standard” will be used here to replace any of the possible tools used such as (with no prejudice to validation of such tool and process to be adequate for the test and pre-conditioning such tools).

X.A-I.7.1 Initial verification at manufacturer’s premises

- a) Test fluid: the use of any substitute fluid for testing shall be validated with fuel comparison data ~~—to~~ assess resulting uncertainties.
- b) Test conditions: environmental conditions (temperature) shall be part of the uncertainty assessment.
- c) Measuring standard ~~-(~~proving cans/verification standards/weighting system): uncertainty and delivery volume to be assessed according to requirement of ~~R-117~~OIML R 117-1, ~~÷~~ 2.5.3.
- d) Sampling and/or split verification (e.g.: separate component check prior to integration in the dispenser). -It is ~~allowed~~ permitted to perform tests at earlier stages of the manufacturing process (for example: ~~—testing~~ 100% of meters individually before integration in dispensers; testing 100% of calculators on simulators; testing 100% of air-separation components on special test bench; testing 100% of SSDs) as long as the manufactured dispensers or SSDs are checked under statistical (minimally 10% of the manufactured population) or systematic survey at the final test.

X.A-I.7.1.1 Administrative verification

- a) Verify the compliance of the design to the type approval certificate/number (reference to the certificate shall be on the type approval plate as per ~~R-117~~OIML R 117-1, ~~—section~~ 2.19.1 and 2.19.2, and on the relevant manufacturer’s ~~ing~~ paperwork).

- b) Check that all the metrological components (e.g., calculator, meter, air separator) are referenced in the type approval certificate.
- c) Check that ~~of~~ the required seals are in place and that they prevent normal dismounting/opening of the associated component (seals do not need to be marked at this time).
- d) Check that the MMQ is clearly indicated for normal conditions of use (see ~~R-117~~R-117OIML R 117-1, ~~section~~ 2.19.1) at dial level.
- e) Check that the identification plate(s) is (are) compliant with the type approval certificate information (or registered design) and include(s) all the markings required in ~~R-117~~R-117OIML R 117-1, ~~section~~ 2.19.
- f) Check that the identification plate(s) is (are) sealed/attached to the dispenser in a durable way.
- g) ~~Record the pass/fail result on the initial verification paperwork~~Record the pass/fail result. In the case of failure, record the reason for the failure.

X.A-I.7.1.2 Accuracy test at high and low ~~flow-rate~~flowrates (testing for fully assembled dispensers)

Note: -If the meters were individually tested before the dispenser assembly, this process shall be described in the manufacturer's quality plan.

- a) Disengage the temperature conversion (if applicable).
- b) Pre-condition the measuring standard.
- c) Lift the nozzle of the EUT, place in the inlet of the measuring standard for high flow, check that the display is reset to zero and stays at zero for 5 seconds, open the nozzle to achieve the maximum ~~flow-rate~~flowrate, perform the accuracy test, and hang the nozzle.
- d) Record the result and the actual flowrate of the test performed.
- e) Check the results versus the MPE requirements of ~~R-117~~R-117OIML R 117-1, ~~section~~ 2.6.1, line A of ~~Table 2~~, and check that the flowrate is between 70 % and 100 % of maximum flowrate of the type approval certificate (see also the identification plate).
- f) Lift the nozzle of the EUT, place in the inlet of the measuring standard -for low flow, check that the display is reset to zero and stays at zero for 5 seconds, open the nozzle to achieve the minimal ~~flow-rate~~flowrate (adjust the flow to stay between 100 % and 120 % of the minimal ~~flow-rate~~flowrate of type approval), perform the accuracy test, and hang the nozzle.
- g) Record the result and the actual flowrate of the test performed.
- h) Check the results versus the MPE requirements of ~~R-117~~R-117OIML R 117-1, ~~section~~ 2.6.1, line A of ~~Table 2~~.
- i) ~~Record the pass/fail result on the initial verification paperwork~~Record the pass/fail result. In the case of failure, record the reason for the failure (if known).

Note: ~~d~~dDuring tests b) and e), the volume of the delivery shall be at least 2 times the MMQ (see ~~R-117~~R-117OIML R 117-1, ~~section~~ 2.5.1).

X.A-I.7.1.3 Accuracy test at MMQ and ~~V~~vapor-recovery check (~~OIML R-117~~OIML R 117-1, Section 2.18.2)

- a) Disengage temperature conversion (if applicable).
- b) Pre-condition the measuring standards (wetting). ~~T~~T—the volume of the test shall be the MMQ.
- c) Disable the increment masking feature at the calculator.

- d) Lift the nozzle of the EUT, place in the measuring standard for MMQ, check that the display is reset to zero and stays at zero for 5 seconds, open the nozzle to achieve the maximum possible ~~flow rate~~flowrate with no spillage, and execute the accuracy test.
- e) For gasoline hoses with vapor recovery: do not hang the nozzle. -Place the nozzle tip out of the measuring standard.- Wait for 2 minutes (or for calculator time out) to witness any unexpected extra increment at the display or any unwanted flow at the nozzle spout. Record the results.
- f) Hang the nozzle.
- g) Record the result of the MMQ check.
- h) Check the results versus the MPE requirements of ~~R-117~~R-117OIML R 117-1 (see ~~R-117~~R-117OIML R 117-1, 2.5.3).
- i) ~~Record the pass/fail result on the initial verification paperwork~~Record the pass/fail result. In the case of failure, record the reason for the failure (if known).

X.A-I.7.1.4 Check of hose dilation and draining (see ~~R-117~~OIML R 117-1, sections 2.13.6 and 2.15)

X.A-I.7.1.4.1 General

The purpose of this section is to check the hose dilation and the nozzle anti-draining device as well as the means to prevent reverse flow to the meter. -All the applicable steps of this section shall be carried out in sequence, with not more than 3 minutes between each sub-section of A.7.1.4.

X.A-I.7.1.4.2 Hose dilation

- a) If an electronic calculator is present, unmask small increments at the display.
- b) Lift the nozzle and do not extend/extract the hose from the dispenser (use actual free reach of the hose) and observe the display for 30 seconds. Read the display after 30 seconds (HD1). Check the volume HD1 against the MPE for hose dilation over MMQ. Record HD1 and MMQ.

X.A-I.7.1.4.3 Draining (procedure from X.A-I.7.1.4.2 continues here)

- a) Place the nozzle spout in a receptacle (any compatible liquid vessel).
- b) Activate the nozzle switch without hanging the nozzle (simulate the nozzle returned to the nozzle boot to terminate the transaction), and observe potential liquid drainage from the nozzle spout for 1 minute.
- c) Release the nozzle boot switch to start a new transaction and observe the display for 30 seconds. The display shall reset first and then the dispenser shall start new transaction. Read the display after 30 seconds (HD2). Check volume HD2 against the MPE for hose dilation over MMQ. Record HD2.
- d) Place the nozzle back in the nozzle boot to terminate the transaction.

X.A-I.7.1.4.4 Hose dilation with hose reel (if applicable, in continuation of X.A-I.7.1.4.3)

- a) While keeping the nozzle in the nozzle boot, uncoil the full length of the hose (on the floor if needed; this action might require special tools such as clamps or locking devices if the hose retractor is automatic).
- b) Lift the nozzle and observe the display for 30 seconds. The display shall reset first and then the dispenser shall start the new transaction. Read the display after 30 seconds (HD3). Check the volume HD3 against the MPE for hose dilation over MMQ. Record HD3.

X.A-I.7.1.4.5 Draining (procedure from X.A-I.7.1.4.4 continues here)

- a) Place the nozzle spout in a receptacle (any compatible liquid vessel).
- b) Activate the nozzle switch without hanging the nozzle (simulate nozzle back in the nozzle boot to terminate the transaction), and observe the potential liquid drainage from the nozzle spout for 1 minute.
- c) Release the nozzle boot switch to start a new transaction and observe the display for 30 seconds. The dDisplay shall reset first and then the dispenser shall start a new transaction. Read the display after 30 seconds (HD4). Check volume HD4 against the MPE for hose dilation over MMQ. Record HD4.
- d) Place the nozzle back in the nozzle boot to terminate the transaction.

X.A-I.7.1.5 Test of the timeout function on dispensers with an electronic indicator (see ~~R-117~~OIML R 117-1, section 5.1.15)

Note: ~~†~~This test only applies to dispensers with electronic indicators. – This test can be replaced by software revision control.

- a) Lift the nozzle to activate the dispenser.
- b) Do not deliver fuel – wait for the timeout.
- c) Check that the dispenser switches off and terminates the transaction within a period not greater than 120 seconds.
- d) Hang the nozzle for 5 seconds.
- e) Lift the nozzle to activate the dispenser.
- f) Deliver a quantity of fuel into the receptacle.
- g) Stop the flow and note the time.
- h) Check that the dispenser switches off and terminates the transaction within a period not greater than 120 seconds.
- i) Hang the nozzle.
- j) Record the result of tests of c) and h).

X.A-I.7.1.6 Air elimination check -- process for fully assembled dispensers

Note: -Adequate air separator individual test upstream manufacturing flow must be integrated in the manufacturer's quality plan.

X.A-I.7.1.6.1 General

- ~~b)a)~~The ~~ss~~suction line connected to the EUT shall be equipped with a suction air-inlet plug with a calibrated inlet hole (example:- between 1.5 and 2.5 mm diameter). The ~~p~~Plug shall be equipped with a control valve to open/close the plug to the atmosphere.
- ~~e)b)p~~Pre-condition the measuring standard – the volume of the check will be 20 ~~liters~~ L minimumal.
- ~~d)c)~~Lift the nozzle of the EUT, place it in the measuring standard~~l~~ for high flow, check that the display is reset to zero and stays at zero for 5 seconds, open the nozzle to achieve maximum possible ~~flow~~ rateflowrate with no spillage, and execute the check.

X.A-I.7.1.6.2 Alternative method 1 – air elimination test with result

- a) ~~D~~uring the flow, open the suction air-inlet plug for 15 seconds (or less if the pump system terminates delivery upon air detection).
- b) ~~h~~Hang the nozzle.
- c) ~~r~~Read the accuracy test result and record the result as air elimination check.
- d) ~~e~~Check the results versus the MPE requirements of ~~R-117~~OIML R 117-1 (take into consideration the viscosity of the fluid or test-fluid in use if applicable) and decide ~~on~~ pass/fail result.

X.A-I.7.1.6.3 Alternative method 2 – air elimination test with blowing evidence

- a) ~~d~~During the flow, open the suction air-inlet plug for 15 seconds (or less if the pump system terminates delivery upon air detection).

- b) ~~e~~Check evidence of air blowing out of air-vent of air-separator.
- c) ~~h~~Hang the nozzle.
- d) ~~i~~If no air-flow was sensed at the air-vent, consider that air-separation has failed.

X.A-I.7.1.6.4 Record pass/fail result on initial verification paperwork-

X.A-I.7.1.7 Ancillary devices

X.A-I.7.1.7.1 Prepay-~~p~~Preset

Purpose of the test: to check that the valve(s) of the dispenser will stop the transaction at the targeted volume with no unacceptable error above the acceptable MPE as per ~~3.6 of R117~~~~R-117~~OIML R 117-1, 3.6. The ~~c~~Check can be simulated or activated by the special calculator menu, or any special control device on the manufacturer's test bench.

~~I~~f the preset function ~~is~~ not available for volume, jump to e).

Set the preset volume to the target check volume (minimum 2 ~~x~~ MMQ). The ~~a~~Amount preset here shall ~~be in~~ correspond~~ence~~ with the measuring standard capacity.

- a) Lift the nozzle to start delivery in the measuring standard. When the delivery is terminated by the dispenser (preset function), hang the nozzle and record the result of the accuracy test and result at the display of the dispenser.
- b) Check the accuracy result ~~versus~~ the MPE requirements of ~~R117~~~~R-117~~OIML R 117-1, ~~(check~~ 3.6.6.)
- c) If the prepay function ~~is~~ not available for the price, jump to i).
- d) Calculate the price prepay target from the measuring standard expected volume (minimum 2 ~~x~~ MMQ). Set the prepay price to the target amount. The ~~a~~Amount preset here shall ~~be in~~ correspond~~ence~~ with the measuring standard -capacity. Some calculation ~~is~~ needed with the price per ~~liter~~litre to ~~be in~~ correspond~~ence~~ with the capacity of the measuring standard. Consider rounding.
- e) Lift the nozzle to start the delivery in the measuring standard. When the delivery is terminated by the dispenser (preset function), hang the nozzle and record the result and display (price, volume and price per ~~liter~~litre).
- f) Check the accuracy versus the MPE requirements of ~~R117~~~~R-117~~OIML R 117-1, ~~(check~~ 3.6.6.)
- ~~-g) Record the pass/fail result on the initial verification paperwork~~Record the pass/fail result.

X.A-I.7.1.7.2 Printer for dispenser

- a) ~~I~~f the dispenser ~~is~~ equipped with its own printer, this check could take place at the time of any previous check.
- b) Check that the ticket issued reflects the information of the display with no allowed difference.
- c) ~~r~~Record the pass/fail result on the initial verification paperworkRecord the pass/fail result.

X.A-I.7.1.8 Temperature conversion (if applicable)

X.A-I.7.1.8.1 General

- ~~E.2a)~~ During the check of the dispensers with the temperature conversion, the special function/menu shall be available to read:

- ~~o~~ Uncompensated volume;
- ~~o~~ temperature of fuel from the EUT probe;
- ~~o~~ Density if applicable;
- ~~o~~ correction tables or parameters, or the signature of ~~the used~~ tables used.

~~E.3b)~~ Proper correction tables or parameters or the signature of the tables to be used shall be made available to the verification operator (e.g., corresponding to the test fluid in use in the factory) so the calibration correction/check can be ~~done~~ carried out properly.

~~E.4c)~~ Proper training is needed for the verification operator to properly assess the results.

~~E.5d)~~ ~~Record the pass/fail result on the initial verification paperwork~~ Record the pass/fail result. In the case of fail, record the reason.

X.A-I.7.1.8.2 ——— Test methods

X.A-I.7.1.8.2.1 General

Temperature conversion when applicable (measurement, probe position, see ~~clauses of OIML R117~~OIML R 117-2, 6.3, and ~~OIML R117~~OIML R 117-1, 6.1.10 note 3.)

X.A-I.7.1.8.2.2 Split EUT verification for first verification

These tests ~~is are performed~~ done to check the accurate temperature reading of fluid in the EUT.

~~F.1a)~~ Install the reference probe (1) at the EUT temperature well.

~~b)~~ Disengage the temperature correction of the EUT.

~~F.2~~ *Note:-* ~~Refer to~~ Refer to the manufacturer's manual as this might be the way to have maintenance information displayed on the EUT dial such as the temperature of the fuel at the EUT conversion probe).

~~F.3c)~~ Run the flow through the EUT at Q_{max} from the storage tank for at least 3 minutes to stabilize the fluid temperature and the EUT temperature (outgoing flow can be re-circulated back to the storage tank).

~~F.4d)~~ Check the accurate temperature reading by comparing the temperature indicated by the EUT (converted signal from its own temperature probe) with ~~the reference~~ reference probe (1) inserted in the temperature well close to the instrument meter/transducer. ~~The m~~Maximum difference allowed is 1.6 °C.

~~F.5e)~~ Stop the flow.

~~F.6f)~~ Check the use of the correct conversion table (as per type approval) in the conversion (calculator) arrangement.

X.A-I.7.1.9 Self-~~s~~Service devices (SSD)

X.A-I.7.1.9.1 Unattended mode – Differed ~~p~~Post payment

When simulation means/tools are used to check ~~s of the~~ the SSD in the factory, the simulation means are most of the time a set of one to several calculators/indicators organized with simulators for volume and other arrangements (nozzle switch, status bulbs for motors/valves). Simulation means can also be fully automated and integrated in one special computer. It is the responsibility of the manufacturer using such simulation tools to fairly demonstrate that his simulation tools are behaving like calculators using the considered protocols.

The test shall verify that correct communication and memorizing/printing is achieved with production instruments.

Example:

- a) Initiate a transaction with the dispenser or simulator (usually, done with a credit card system).
- b) Activate a few ~~liter~~litres of flow, and hang the nozzle.
- c) Check the good transmission of the corresponding transaction to the SSD.
- d) Compare the display of the dispenser with the memorized (or printed when applicable) information at the SSD. This check can also be conducted ~~also~~ on the ticket printer at the credit card payment terminal when applicable.
- e) Check the good retrieving of the last transaction from the SSD memory when applicable.
- ~~-f) Record the pass/fail result on the initial verification paperwork~~Record the pass/fail result.

X.A-I.7.1.9.2 Attended mode – Temporary storage mode – Immediate ~~P~~post payment

When simulation means/tools are used during checks of the SSD in the factory, the simulation means are most of the time a set of one to several calculators/indicators organized with simulators for volume and other arrangements (nozzle switch, status bulbs for motors/valves). Simulation means can also be fully automated and integrated in one special computer. It is the responsibility of the manufacturer using such simulation tools to fairly demonstrate that his simulation tools are behaving like calculators using the considered protocols.

The test shall verify that correct the communication and memorizing/printing is achieved with production instruments.

- ~~-a)~~ Initiate a transaction with the EUT.
- b) Activate a few ~~liter~~litres of flow, and hang the nozzle.
- ~~-c)~~ Initiate a new transaction with the EUT.
- d) Activate a few ~~liter~~litres of flow (different volume from the first transaction), and hang the nozzle.
- ~~-e)~~ Try to initiate a new transaction with the EUT – it must be impossible (limited stacking to 2 transactions).
- f) Check the good transmission of the corresponding transactions to the console/SSD.
- g) Check the good retrieving of both transactions from the SSD memory when applicable.
- h) ~~Record the pass/fail result on the initial verification paperwork~~Record the pass/fail result. In case of fail, record the reason.

X.A-I.7.2 Initial verification on demand, at place of use

X.A-I.7.2.1 General

- ~~-a) T~~est fluid: dispensers are tested with fuel to be dispensed.
- b) ~~T~~est conditions: environmental conditions (temperature) to be part of uncertainty assessment, as well as evaporation, wind, misting and potential denting of measuring standards.
- c) ~~m~~Measuring standard : uncertainty and volume of checks to be assessed according to requirements of ~~R-117~~R-117OIML R 117-1:2014:2.5.3

X.A-I.7.2.2 Administrative test

- a) Verify the compliance of the design to the type approval certificate (the reference of the certificate is expected on the type approval plate).
- b) Check that all known metrological components (e.g., calculator, meter, air separator) are referenced in the type approval certificate.
- c) Check that the relevant seals are in place and preventing normal dismounting/opening of the associated component (seals do not need to be marked at this time).
- d) Check that the MMQ is properly indicated at the dial level.
- e) Check that the identification plate(s) is (are) compliant with the type certificate information (or registered design).
- f) Check that the identification plate(s) is (are) sealed/attached to the dispenser in a durable way.
- g) ~~Record the pass/fail result on the initial verification paperwork~~Record the pass/fail result. In the case of fail, record the reason if known.

X.A-I.7.2.3 Accuracy test at high and low flow

- a) Disengage the temperature conversion if applicable.
- ~~-b)~~ Pre-condition measuring standards.
- c) Lift the nozzle of the EUT, place it in the measuring standard for high flow, check that the display is reset to zero and stays at zero for 5 seconds, open the nozzle to achieve maximum ~~flow-rate~~flowrate, carry -out the accuracy test, and hang the nozzle.
- d) Record the result, and ~~real-the real~~ flowrate.
- e) Check the results versus the MPE requirements of ~~R-117~~R-117OIML R 117-1, and check that the flowrate is between 50% and 100% of the maximum flowrate of the type certificate (see also the identification plate).
- f) Lift the nozzle of the EUT, place it in the measuring standard for low flow, check that the display is reset to zero and stays at zero for 5 seconds, open the nozzle to achieve minimal ~~flow-rate~~flowrate (adjust during flow to stay between 100% and 120% of the minimal ~~flow-rate~~flowrate of the type approval), carry -out the accuracy test, and hang the nozzle.
- g) Record the result, and the real flowrate.
- h) Check the results versus the MPE requirements of ~~R-117~~R-117OIML R 117-1.
- i) ~~Record the pass/fail result on the initial verification paperwork~~Record the pass/fail result. In the case of fail, record the reason if known.

X.A-I.7.2.4 Accuracy test at MMQ and ~~h~~Hose check

- a) Disengage the temperature conversion if applicable.
- b) Pre-condition the measuring standard – the volume of the check will be the MMQ.
- c) Disable the increment masking feature at the calculator.
- d) Lift the nozzle of the EUT, place it in the measuring standard for high flow, check that the display is reset to zero and stays at zero for 5 seconds, open the nozzle to achieve maximum possible ~~flow-rate~~flowrate with no spillage, carry -out the accuracy test.
- e) For gasoline hoses, with vapour recovery: do not hang the nozzle but keep the nozzle spout out of the measuring standard. Wait for the calculator time out (or one minute) to witness any unexpected extra increment at display. Record the result. Unexpected extra increments at the display shall not exceed 1% of MMQ.

- f) Hang the nozzle.
- ~~-g)~~ Record the result of the MMQ accuracy check.
- h) Check the results versus the MPE requirements of ~~R-117~~OIML R 117-1 (see ~~R-117~~OIML R 117-1, 2.5.3).
- i) ~~Record the pass/fail result on the initial verification paperwork~~Record the pass/fail result. In the case of fail, record the reason if known.

FOR

X.A-I.7.2.5 Test of the timeout function on dispensers with electronic indicator (see ~~R-117~~OIML R 117-1, ~~section 5.1.15~~) – this test can be replaced by software revision control.

Note: ~~€~~This test only applies to dispensers with electronic indicators.

- a) Lift the nozzle to activate the dispenser.
- b) ~~D~~eo not deliver fuel – wait for timeout.
- c) ~~e~~Check that the dispenser switches off and terminates the transaction within a period not greater than 120 seconds.
- d) Hang the nozzle for 5 seconds.
- e) Lift the nozzle to activate the dispenser.
- f) ~~D~~eliver a quantity of fuel into the receptacle.
- g) Stop the flow and note the time.
- h) ~~e~~Check that the dispenser switches off and terminates the transaction within a period not greater than 120 seconds.
- i) ~~h~~Hang the nozzle.
- j) ~~R~~Record the result of the test of c) and h).

X.A-I.7.2.6 Air elimination check

X.A-I.7.2.6.1 General

The s~~S~~uction line or inlet connected to the EUT shall be equipped with a suction air-inlet plug with a calibrated inlet hole between 1.5 and 2.5 mm in diameter. The p~~p~~lug shall be equipped with a control valve to open/close the plug to the atmosphere. ~~It must be such that it may~~ ~~Such can~~ be connected to any drain plug or fitted on a special cover (e.g. special test inlet filter cover). This special air-inlet can be removed after verification on site is ~~done~~finished. -When done on site, this test creates a hazardous situation. Operators shall be properly trained with respect to “explosion safety” rules and precautions.

X.A-I.7.2.6.2 ~~Alternative~~Alternative method 1 – air elimination test with result

- a) ~~D~~during the accuracy test, open the suction air-inlet plug for 15 seconds.
- b) ~~H~~Hang the nozzle.
- a)c) ~~R~~Record the accuracy result with ~~of~~ air.
- b)d) ~~C~~Check the results versus the MPE requirements of ~~R-117~~OIML R 117-1 (take into consideration the viscosity of the fluid or test ~~-~~fluid in use if applicable).

X.A-I.7.2.6.3 ~~Alternative~~Alternative method 2 - -air elimination test with blowing evidence

- a) During a test run in a ~~receptable~~receptacle, open the suction air-inlet plug for 15 seconds.
- b) Check evidence of air blowing out of the air-vent of the air-separator.
- c) Hang the nozzle.
- d) If no air-flow was sensed at the air-vent, consider that air-separation has failed.
- ~~-e) Record the pass/fail result on the initial verification paperwork~~Record the pass/fail result.

X.A-I.7.2.7 Ancillary devices

X.A-I.7.2.7.1 Prepay

- a) ~~C~~heck ~~of the~~ prepay function of ~~the~~ dispenser. ~~The c~~Check must be activated from ~~the~~ console controlling ~~the~~ site.
- b) Set ~~the~~ prepay volume to the target check volume (minimum 2 ~~x~~ MMQ) – to be done at ~~the~~ kiosk of ~~the~~ station.
- c) Activate at ~~the~~ console, walk back to ~~the~~ dispenser and carry out ~~the~~ accuracy test, record ~~the~~ result.
- d) Check ~~the~~ result versus ~~the~~ MPE requirements of ~~R-117~~~~R-117~~OIML R 117-1.
- e) ~~R~~ecord ~~the~~ pass/fail result. In ~~the~~ case of fail, record ~~the~~ reason if known.

X.A-I.7.2.7.2 Printer for dispenser

- a) ~~I~~f ~~the~~ dispenser ~~is~~ equipped with its own printer, ~~the~~ check could take place during any previous check.
- b) Check that ~~the~~ ticket issued reflects ~~the~~ information of ~~the~~ dial with no allowed difference.
- ~~c) ~~R~~ecord ~~the~~ pass/fail result on ~~the~~ initial verification paperwork~~Record the pass/fail result.

X.A-I.7.2.8 Temperature conversion (if applicable)

X.A-I.7.2.8.1 General

- a) During ~~the~~ check of ~~the~~ dispensers with temperature conversion, ~~the~~ special function/menu shall be available to read:
 - o ~~U~~ncompensated volume.
 - o ~~t~~emperature of fuel from EUT probe.
 - o ~~D~~ensity if applicable.
 - o ~~the c~~Correction tables or parameters, or ~~the~~ signature of ~~the used~~ tables ~~used~~.
- b) Proper correction tables or parameters or signature of tables to be used shall be made available to the verification operator (e.g. ~~:-~~corresponding to ~~the~~ test fluid in use in ~~the~~ factory) so ~~that the~~ calibration correction/check can be done properly.
- c) Proper training is needed for ~~the~~ verification operator to properly assess ~~the~~ results.

X.A-I.7.2.8.2 Test methods

X.A-I.7.2.8.2.1 -General

Temperature conversion when applicable (measurement, probe position, see ~~clauses~~ of ~~OIML~~ ~~R-117~~~~R-117~~OIML R 117-2, 6.3, and ~~OIML~~ ~~R-117~~~~R-117~~OIML R 117-1, 6.1.10, note 3).

X.A-I.7.2.8.2.2 Split EUT verification for first verification

These tests ~~are~~is done to check ~~the~~ accurate temperature reading of ~~the~~ fluid in ~~the~~ EUT.

- a) Install ~~the~~ reference probe (1) at ~~the~~ EUT temperature well.

b) Disengage the temperature correction of the EUT.

d) *Note:* ~~Refer to~~ the manufacturer's manual as this might be the way to have maintenance information displayed on the EUT dial such as the temperature of the fuel at the EUT conversion probe).

e) Run the flow through the EUT at Q_{\max} from the storage tank for at least 3 minutes to stabilize the fluid temperature and the EUT temperature (outgoing flow can be re-circulated back to the storage tank).

f) Check the accurate temperature reading by comparing the temperature indicated by the EUT (converted signal from its own temperature probe) with the ~~reference~~ reference probe (1) inserted in the temperature well close to the instrument meter/transducer. The ~~m~~ maximum difference allowed is 1.6 °C.

g) Stop the flow.

h) Check the use of the correct conversion table (as per the type approval) in the conversion (calculator) arrangement.

X.A-I.7.2.9 Self-~~S~~service devices

X.A-I.7.2.9.1 Unattended mode – Differed ~~p~~Post payment

- Initiate a transaction with the connected dispenser (usually, done with a credit card system).
- Activate a few ~~liter~~litres of flow, and hang the nozzle.
- Check the good transmission of the corresponding transaction to the SSD.
- Compare the display of the dispenser with the memorized (or printed when applicable) information at the SSD. This check can also be conducted ~~also~~ on the ticket printer at the credit card payment terminal when applicable.
- Check the good retrieving of the last transaction from the SSD memory when applicable.
- ~~Record the pass/fail result on the initial verification paperwork~~Record the pass/fail result. In the case of fail, record reason.

X.A-I.7.2.9.2 Attended mode – Temporary storage mode – Immediate ~~p~~Post payment

- Initiate a transaction with the EUT.
- Activate a few ~~liter~~litres of flow, and hang the nozzle.
- ~~b) c)~~Initiate a new transaction with the EUT.
- Activate a few ~~liter~~litres of flow (different volume from the first transaction), and hang the nozzle.
- ~~e) e)~~Try to initiate a new transaction with the EUT – it must be impossible (limited stacking to 2 transactions).
- Check the good transmission of the corresponding transactions to the console/SSD.
- Check the good retrieving of both transactions from the SSD memory when applicable.
- ~~Record the pass/fail result on the initial verification paperwork~~Record the pass/fail result. In the case of fail, record the reason.

Annex X.A-LPG

Testing procedures (initial verification) for LPG dispensers

Definitions for the purpose of this Annex

Note to reader: (These could migrate to the beginning of R117R-117-2 after review)

Dynamic flow corrected meters: a meter associated with its transducer, where correction factors linked to ~~the flow rate~~flowrate are used to adjust the measurement dependently (2 or more factors to optimized the accuracy curve of the measuring system over the ~~flow rate~~flowrate range).

Measuring standard: generic term to designate the adequate tools (and process) in use to check the accuracy of the instrument/meter (see note 2). Special care shall be taken to properly assess the ratio of the mix of ~~b~~Butane and ~~P~~Propane in use for any test if it can influence the accuracy of the measuring standards.

Console: an ancillary device control system, not in the scope of the type certification, capable of setting the unit price to the dispenser and controlling various phases in self-serving mode on petrol stations (releasing a dispenser, cash ~~-~~in a dispenser, stop a dispenser, changing price of LPG fuel) using the communication protocol with the dispenser calculator.

LPG dispenser: ~~-~~are considered as LPG dispensers in this ~~a~~Annex all commonly used fuel or liquid dispensers where the liquid has a saturating vapor pressure above atmospheric pressure at ambient temperature (~~example is e.g.~~ DMF). This includes ~~s~~d equipment on petrol stations and also used to feed boats s or small aircraft, when the operation of these is done “hose full”.

X.A-L-I.7 General information for initial verification – Preamble

Initial verification of fuel dispensers is the responsibility of national authorities, and may be done either:

- ~~-a)~~ Aat the factory of the manufacturer;
- ~~-b)~~ under quality insurance control, if permitted by the national authority of the country of use;
- ~~-c)~~ by inspection of the apparatus, routine or batch sample, as per the regulations of the country of use, done by the authorized inspection organization;
- ~~-d)~~ Aat the site of use. Common practice is for national authorities to perform this, unless it is subcontracted to an approved/authorized representative of the manufacturer or authority.

Note: ~~-~~The expression “measuring standard” will be used here to replace any of the possible tools used such as (with no prejudice to validation of such tool and process to be adequate for the test and pre-conditioning such tools).

X.A-L-I.7.1 Initial verification at manufacturer’s premises

- ~~2)a)~~ Test fluid: the use of any substitute fluid for testing shall be validated with fuel comparison data— to assess resulting uncertainties.
- ~~3)b)~~ Test conditions: environmental conditions (temperature) ~~to~~shall be part of the uncertainty assessment.
- ~~4)c)~~ Measuring standard ~~-(~~proving cans/verification standards/weighting system): uncertainty and delivery volume are to be assessed according to the requirement of ~~R-117~~R-117OIML R 117-1, ÷ 2.5.3.
- ~~5)d)~~ Sampling and/or split verification (e.g. ÷ separate component check prior to integration in the dispenser). ~~-~~It is allowed to perform tests at the earlier stages of the manufacturing process (e.g. ÷ testing 100% of ~~-~~meters individually before integration in the dispensers, testing 100% of the

calculators on simulators, testing 100% of air-separation on a special test bench, testing 100% of SSDs) as long as the manufactured dispensers or SSDs are checked under a statistical (minimal 10% of manufactured population) or systematic survey at the final test.

X.A-L-I.7.1.1 Administrative verification

- ~~5)a)~~ Verify the compliance of the design to the type approval certificate/number (reference to the certificate shall be on the type approval plate as per ~~R-117~~R-117OIML R 117-1, ~~section~~-2.19.1 and 2.19.2, and on the manufacturer's relevant paperwork).
- ~~6)b)~~ Check that all the metrological components (e.g. the calculator, meter, air separator when applicable) are referenced in the type approval certificate.
- ~~7)c)~~ Check that the required seals are in place and preventing normal dismounting/opening of the associated component (seals do not need to be marked at this time).
- ~~8)d)~~ Check that the MMQ is clearly indicated in normal conditions of use (see ~~R-117~~R-117OIML R 117-1, ~~section~~ 2.19.1) at the dial level.
- ~~9)e)~~ Check that the identification plate(s) is (are) compliant with the type approval certificate information (or registered design) and contain the markings required in ~~R-117~~R-117OIML R 117-1, ~~section~~ 2.19.
- ~~10)f)~~ Check that the identification plate(s) is (are) sealed/attached to the dispenser in a durable way.
- ~~11)g)~~ ~~Record the pass/fail result on the initial verification paperwork~~ Record the pass/fail result. In the case of fail, record the reason.

X.A-L-I.7.1.2 Accuracy test at high and low flow – process for fully assembled dispensers

Note: If the meters are individually tested before the dispenser assembly, this process shall be fully described in the manufacturer's quality plan.

An adequate individual meter ~~individual~~ test upstream of the manufacturing flow must be integrated in the manufacturer's quality plan.

- ~~a)~~ Disengage the temperature conversion if applicable.
- ~~b)~~ Pre-condition the measuring standard.
- ~~c)~~ Lift the nozzle of the EUT, place the nozzle in the in-inlet of the measuring standard for high flow, check that the display is reset to zero and stays at zero for 5 seconds, activate the flow (dead man push button if needed) to achieve maximum ~~flow-rate~~flowrate, carry out the accuracy test, and hang the nozzle.
- ~~d)~~ Record the result, and the actual flowrate of the test done.
- ~~e)~~ Check the results versus the MPE requirements of ~~R-117~~R-117OIML R 117-1, ~~section~~ 2.6.1 line A of ~~Table~~ 2, and check that the flowrate is between 80% and 100% of the maximum flowrate of the type certificate (see also the identification plate).
- ~~f)~~ Set the flow valve arrangement (e.g. the valve between the nozzle and the hose) for low flow.
- ~~g)~~ Lift the nozzle of the EUT, place the nozzle in the inlet of the measuring standard -for low flow, check that the display is reset to zero and stays at zero for 5 seconds, activate the flow (dead man push button if needed)- to achieve minimal ~~flow-rate~~flowrate (adjust during the flow to stay between 100% and 120% of the minimal ~~flow-rate~~flowrate of the type approval), carry out the accuracy test, and hang the nozzle.
- ~~h)~~ Record the result, and the actual flowrate of the test done.

- i) ~~e~~Check the results versus the MPE requirements of ~~R-117~~R-117OIML R 117-1, ~~section~~ 2.6.1 line A of ~~Table 2~~.
- j) ~~Record the pass/fail result on the initial verification paperwork~~Record the pass/fail result. In the case of fail, record the reason if known.

Note: ~~d~~During tests b) and e), the volume of delivery shall be at least 2 times the MMQ (see ~~R-117~~R-117OIML R 117-1, ~~section~~ 2.5.1).

X.A-L-I.7.1.3 Accuracy test at MMQ

- 1)a) Disengage the temperature conversion if applicable.
- 2)b) ~~p~~Pre-condition the measuring standards – the volume of the test shall be MMQ.
- 3)c) Disable the increment masking feature at the calculator.
- 4)d) ~~Lift~~ Lift the nozzle of the EUT, connect the nozzle to the measuring standard for the MMQ, check that the display is reset to zero and stays at zero for 5 seconds, activate the flow to achieve the maximum possible ~~flow-rate~~flowrate, execute the accuracy test.
- 5)e) Hang the nozzle.
- f) Record the result of the MMQ check.
- 6)g) ~~Check~~ Check the results versus the MPE requirements of ~~R-117~~R-117OIML R 117-1, ~~(see R-117-1: 2.5.3.)~~
- 7)h) ~~Record the pass/fail result on the initial verification paperwork~~Record the pass/fail result. In the case of fail, record the reason if known.

X.A-L-I.7.1.4 Check of hose dilation and draining (see ~~R-117~~R-117OIML R 117-1, ~~sections 2.13.6 and 2.15~~)

X.A-L-I.7.1.4.1 General

The purpose of this section is to check the hose dilation and nozzle anti-draining device as well as the means to prevent reverse flow to the meter. All the applicable steps of this section shall be carried out in sequence, with not more than 3 minutes between each sub-sections of X.A-L-I.7.1.4.

X.A-L-I.7.1.4.2 Hose dilation

- a) ~~if~~ if ~~the electronic~~ calculator is electronic, unmask the small increments at display.
- b) ~~Lift~~ Lift the nozzle and do not extend/extract the hose from the dispenser (use the actual free reach of the hose), activate the flow while the nozzle is not connected (dead man push button if needed) –and observe the display for 30 seconds. Read the display after 30 seconds (HD1). Check the volume HD1 against the MPE for the hose dilation over the MMQ. Record HD1 and MMQ.
- c) Release the dead man push button.

X.A-L-I.7.1.4.3 Draining (procedure from A.7.1.4.2 continues here)

- 5)a) ~~C~~connect the nozzle to the storage return line (or any compatible liquid vessel).
- 6)b) ~~a~~Activate the nozzle switch without hanging the nozzle (simulate the nozzle back in the nozzle boot to terminate the transaction), and observe any potential liquid drainage from the nozzle spout for ~~1~~1 minute.
- 7)c) Release the nozzle boot switch to start a new transaction and observe the display for 30 seconds. ~~The~~ dDisplay shall reset first and then the dispenser shall start a new transaction. Read the display after ~~30~~

30 seconds (HD2). Check the volume HD2 against the MPE for the hose dilation over the MMQ. Record HD2.

~~8)d)~~ Place the nozzle back in the nozzle boot to terminate the transaction.

X.A-L-I.7.1.4.4 Hose dilation with hose reel (if applicable, in continuation of A.7.1.4.3)

- a) ~~W~~While keeping the nozzle in the nozzle boot, uncoil the hose full length (on the floor if needed; this action might require special tools such as clamps or locking devices if the hose retractor is automatic).
- b) Lift the nozzle, but do not connect ~~nozzle it~~. Activate the flow (dead man push button if needed) and observe the display for 30 seconds. The ~~d~~Display shall reset first and then the dispenser shall start the new transaction. Read the display after 30 seconds (HD3). Check the volume HD3 against the MPE for the hose dilation over the MMQ. Record HD3.

X.A-L-I.7.1.4.5 Draining (procedure from A.7.1.4.4 continues here)

- ~~a)~~ eConnect the nozzle to the storage return line (or any compatible liquid vessel).
- ~~b)~~ aActivate the nozzle switch without hanging the nozzle (simulate the nozzle back in the nozzle boot to terminate the transaction), and observe any potential liquid drainage from the nozzle spout for ~~1~~ 1 minute.
- ~~c)~~ Release the nozzle boot switch to start a new transaction and observe the display for 30 seconds. The ~~d~~Display shall reset first and then the dispenser shall start a new transaction. Read the display after ~~30~~ 30 seconds (HD2). Check the volume HD2 against the MPE for the hose dilation over the MMQ. Record HD2.
- ~~d)~~ pPlace the nozzle back in the nozzle boot to terminate the transaction.

X.A-L-I.7.1.5 Test of timeout function on dispensers with electronic indicator (see ~~R-117~~R-117OIML R 117-1, section 5.1.15)

Note 1: This test can be replaced by software revision control.

Note 2: ~~1~~ This test only applies to dispensers with electronic indicators.

- ~~4)a)~~ Lift the nozzle to activate the dispenser.
- ~~5)b)~~ do not deliver any fuel – wait for timeout.
- ~~6)c)~~ eCheck that the dispenser switches off and terminates the transaction within a period not greater than 120 seconds.
- ~~7)d)~~ Hang the nozzle for 5 seconds.
- ~~8)e)~~ Lift the nozzle to activate the dispenser.
- ~~f)~~ Connect the nozzle to the storage tank return line and deliver a quantity of fuel.
- ~~9)g)~~ Stop the flow and note the time.
- ~~10)h)~~ eCheck that the dispenser switches off and terminates the transaction within a period not greater than 120 seconds.
- ~~11)i)~~ hang the nozzle.
- ~~12)j)~~ record the result of the tests of c) and h).

X.A-L-I.7.1.6 Air elimination check - process for fully assembled dispensers

Warning note: ~~T~~h~~i~~s test can only be achieved with actual LPG fuel. If a low saturating pressure substitute fluid is used, this test shall be adjusted, see note (below).

- a) ~~The~~ l~~i~~q~~u~~i~~d~~ pressurized line connected to the EUT shall enter the EUT via an electric controlled valve, activated by the operator's request for flow (dead man push button if needed).
- b) During the idle state, the remaining liquid LPG is allowed to boil back to the storage tank via the storage tank return line for safety reasons. The ~~p~~u~~r~~p~~o~~s~~e~~ of this test is ~~t~~o make sure that the volume of LPG under the gaseous phase will not alter the accuracy of t~~h~~e measuring system at the next transaction.
- c) ~~p~~r~~e~~-condition the measuring standard – volume of check will be 20 ~~liters~~L minimal.
- d) Leave the EUT idle for 3 minutes (relaxing time for air-separator to boil the liquid back to the storage tank).
- e) ~~L~~i~~f~~t the nozzle of the EUT while keeping the nozzle switch of the boot activated (to prevent pump activation), connect to ~~the~~ measuring standard f~~o~~r high flow.
- f) Activate the flow, ~~simultaneously~~s~~im~~u~~ltaneousises releasing the nozzle boot switch. ~~e~~c~~heck that the display is reset to zero and stays at zero for 5 seconds, activate the flow immediately to achieve the maximum possible ~~flow-rate~~flowrate with no spillage. ~~E~~x~~e~~cute the accuracy check. The ~~r~~e~~su~~lt shall be within the MPE for air-elimination.~~~~~~~~

Note: ~~i~~f using a low saturating pressure substitute fluid, step d) is replaced by step d') (as follows):

~~d)~~ f~~l~~u~~sh the air separator with nitrogen at high flow so that the liquid inside the air separator is expelled back to the storage tank.~~

X.A-L-I.7.1.7 Ancillary devices

X.A-L-I.7.1.7.1 Prepay-~~P~~preset (when applicable)

Purpose of the test: to check that the valve(s) of the LPG dispenser will stop the transaction at the targeted volume with no unacceptable error above the acceptable MPE as per ~~3.6 of R-117~~R-117~~OIML R 117-1, 3.6.~~ The ~~c~~c~~h~~eck can be simulated or activated by the special calculator menu, or any special control device on the manufacturer's test bench.

- a) If the preset function is not available for volume, jump to e).
- b) Set the preset volume to the target check volume (minimum 2 ~~xx~~ MMQ). The ~~A~~amount preset here shall ~~be in~~correspondence with the measuring standard capacity.
- c) Connect the nozzle to start the delivery in the measuring standard. When the delivery is terminated by the dispenser (preset function), hang the nozzle and record the result of the accuracy test and the result at the display of the dispenser.
- d) Check the accuracy result- versus the MPE requirements of ~~R-117~~R-117~~OIML R 117-1, (check 3.6.6.)~~
- e) If the prepay function not available for price, jump to i).
- f) Calculate the price prepay target from the measuring standard expected volume (minimum 2 ~~xx~~ MMQ). Set the prepay price to the target amount. The ~~a~~amount preset here shall ~~be in~~correspondence with the measuring standard -capacity. Some calculation is needed with the price per literlitre to ~~be in~~correspondence with the capacity of the measuring standard. Consider rounding.
- g) Lift the nozzle to start the delivery in the measuring standard. When the delivery is terminated by the dispenser (preset function), hang the nozzle and record the result and the display (price, volume and price per literlitre).
- h) Check the accuracy versus the MPE requirements of ~~R-117~~R-117~~OIML R 117-1, (check 3.6.6.)~~

~~-i) Record the pass/fail result on the initial verification paperwork~~Record the pass/fail result.

X.A-L-I.7.1.7.2 Printer for dispenser

~~-a) If the~~ dispenser is equipped with its own printer, this check could take place at the time of any previous check.

~~-b)~~ Check that the ticket issued reflects the information of the display with no allowed difference.

~~-c) Record the pass/fail result on the initial verification paperwork~~Record the pass/fail result.

EDITOR

X.A-L-I.7.1.8 Temperature conversion (if applicable)

X.A-L-I.7.1.8.1 General

- a) During the check of the LPG -dispensers with temperature conversion, the special function/menu shall be available to read
 - o the ~~U~~uncompensated volume,
 - o the ~~t~~Temperature of the LPG fuel from the EUT probe,
 - o the ~~d~~Density if applicable, and
 - o the ~~c~~Correction tables or parameters, or the signature of ~~used~~ tables used.
- b) Proper correction tables or parameters or signature of tables to be used shall be made available to the verification operator (e.g., corresponding to the test fluid in use in the factory) so that the calibration correction/check can be done properly.
- c) Proper training is needed for the verification operator to properly assess the results.
- d) ~~Record the pass/fail result on the initial verification paperwork~~Record the pass/fail result. In the case of fail, record the reason.

X.A-L-I.7.1.8.2 Test methods

X.A-L-I.7.1.8.2.1 General

Temperature conversion when applicable (measurement, probe position, see ~~clauses of OIML R-117~~~~OIML R 117-2~~, 6.3, and ~~OIML R-117~~~~OIML R 117-1~~, 6.1.10 note 3).

X.A-L-I.7.1.8.2.2 Split EUT verification for first verification

These tests ~~is~~~~are carried out done~~ to check the accurate temperature reading of the fluid in the EUT

- a) Install the reference probe (1) at the EUT temperature well.
- b) Disengage the temperature correction of the EUT (*Note:* refer to the manufacturer's manual as this might be the way to have maintenance information displayed on the EUT dial such as the temperature of the LPG fuel at the EUT conversion probe).
- c) Connect the nozzle to the storage tank return line. Run the flow through the EUT at Q_{\max} from the storage tank for at least 3 minutes to stabilize the fluid temperature and the EUT temperature (the outgoing flow can be re-circulated back to the storage tank).
- d) Check the accurate temperature reading by comparing the temperature indicated by the EUT (converted signal from its own temperature probe) with the reference ~~reference~~ probe (1) inserted in the temperature well close to the instrument meter/transducer. ~~The m~~~~M~~maximum difference allowed is 1.3-3 °C.
- e) Stop the flow.
- f) Check the use of the correct conversion table (as per the type approval) in the conversion (calculator) arrangement.

X.A-L-I.7.1.9 Self Service devices (SSD)

X.A-L-I.7.1.9.1 Unattended mode – Differed ~~P~~post payment

When the simulation means/tools are used to check ~~s of the~~ SSD in the factory, the simulation means are most of the time a set of one to several calculators/indicators organized with the simulators for volume and other arrangements (nozzle switch, status bulbs for motors/valves). The ~~s~~Simulation means can also be fully automated and integrated in one special computer. It is the responsibility of the manufacturer using such simulation tools to fairly demonstrate that his simulation tools are behaving like calculators using the considered protocols.

The test shall verify that correct communication and memorizing/printing is achieved with production instruments.

Example:

- a) Initiate a transaction with the EUT (usually, done with a credit card system).
- b) Activate a few ~~liter~~litres of flow, and hang the nozzle.
- c) Check the good transmission of the corresponding transaction.
- d) Compare the display of the dispenser with the memorized (or printed when applicable) information at the SSD. This check can also be conducted ~~also~~ on the ticket printer at the credit card payment terminal when applicable.
- e) Check the good retrieving of the last transaction for the SSD memory when applicable.
- f) ~~Record the pass/fail result on the initial verification paperwork~~Record the pass/fail result.

X.A-L-I.7.1.9.2 Attended mode – Sale stacking – Immediate ~~P~~post payment

When the simulation means/tools are used ~~during to~~ checks ~~s of the~~ SSD in the factory, the simulation means are most of the time a set of one to several calculators/indicators organized with the simulators for volume and other arrangements (nozzle switch, status bulbs for motors/valves). The ~~s~~Simulation means can also be fully automated and integrated in one special computer. It is the responsibility of the manufacturer using such simulation tools to fairly demonstrate that his simulation tools are behaving like calculators using the considered protocols.

The test shall verify that correct communication and memorizing/printing is achieved with production instruments.

- a) Initiate a transaction with the EUT.
- b) Activate a few ~~liter~~litres of flow, and hang the nozzle.
- c) Initiate a new transaction with the EUT.
- d) Activate a few ~~liter~~litres of flow (different volume from the first transaction), and hang the nozzle.
- e) Try to initiate a new transaction with the EUT – it must be impossible (limited stacking to 2 transactions).
- f) Check the good transmission of the corresponding transactions to the console/SSD.
- g) Check the good retrieving of both the transactions from the SSD memory when applicable.
- h) ~~Record the pass/fail result on the initial verification paperwork~~Record the pass/fail result. In the case of fail, record the reason.

X.A-L-I.7.2 Initial verification on demand, at place of use

X.A-L-I.7.2.1 General

- a) ~~T~~est fluid: the dispensers are tested with the fuel to be dispensed.

- b) ~~Test~~ conditions: the environmental conditions (temperature) are to be part of the uncertainty assessment, as well as evaporation, wind, misting and potential denting of measuring standards.
- c) ~~Measuring standard~~:- the uncertainty and the volume of checks are to be assessed according to the requirement of ~~R-117~~R-117OIML R 117-1÷, 2.5.3.

X.A-L-I.7.2.2 Administrative test

- a) Verify the compliance of the design to the type approval certificate (the reference of the certificate is expected on the type approval plate).
- b) Check that all known metrological components (e.g. calculator, meter, air separator) are referenced in the type approval certificate.
- c) Check that the relevant seals are in place and preventing normal dismounting/opening of the associated component (seals do not need to be marked at this time).
- d) Check that the MMQ is properly indicated at the dial level.
- e) Check that the identification plate(s) is (are) compliant with the type certificate information (or the registered design).
- f) Check that the identification plate(s) is (are) seals/attached to the dispenser in a durable way.
- g) ~~Record the pass/fail result on the initial verification paperwork~~Record the pass/fail result. In the case of fail, record the reason if known.

X.A-L-I.7.2.3 Accuracy test at high and low flow

- a) Disengage the temperature conversion if applicable.
- b) Pre-condition the measuring standards.
- c) Lift the nozzle of the EUT, connect the nozzle to the measuring standard for high flow, check that the display is reset to zero and stays at zero for 5 seconds, open the nozzle to achieve maximum ~~flow~~ rateflowrate, carry-out the accuracy test, and hang the nozzle.
- d) Record the result, and the real flowrate.
- e) Check the results versus the MPE requirements of ~~R-117~~R-117OIML R 117-1, and check that the flowrate is between 50 % and 100 % of the maximum flowrate of the type certificate (see also the identification plate).
- f) Lift the nozzle of the EUT, connect it to the -measuring standard for low flow (see note), check that the display is reset to zero and stays at zero for 5 seconds, open the nozzle to achieve minimal ~~flow~~ rateflowrate (adjust during flow to stay between 100 % and 120 % of minimal ~~flow rate~~ flowrate of the type approval), carry-out the accuracy test, and hang the nozzle.
- g) Record the result, and the real flowrate.
- h) Check the results versus the MPE requirements of ~~R-117~~R-117OIML R 117-1.
- i) ~~Record the pass/fail result on the initial verification paperwork~~Record the pass/fail result. In the case of fail, record the reason if known.

Note 1: To adjust the low flow, the operation might require a special adjusting valve at the entry port of the measuring standard to avoid modifications to the EUT hose/nozzle arrangement.

Note 2: The target of 50 % of point e) might be difficult to match on site with the temperature of vapours in the receiving tank.

X.A-L-I.7.2.4 Accuracy test at MMQ (if applicable) and ~~h~~Hose check

- ~~a~~) Disengage temperature conversion if applicable.
- ~~b~~) Pre-condition measuring standard – volume of check will be MMQ.
- ~~c~~) Disable increment masking feature at calculator.
- ~~d~~) Lift nozzle of EUT, connect to measuring standard for high flow, check that display is reset to zero and stays at zero for 5 seconds, activate flow (e.g.: dead man push button), carry-out accuracy test.
- ~~e~~) Hang nozzle.
- ~~f~~) Record result of MMQ accuracy check.
- ~~g~~) Check results versus MPE requirements of ~~R-117~~OIML R 117-1 (see ~~R-117~~OIML R 117-1: 2.5.3).
- ~~h~~) Record pass/fail result on initial verification paperwork. In case of fail, record reason if known.

X.A-L-I.7.2.5 Test of timeout function on dispensers with electronic indicator (see ~~R-117~~OIML R 117-1, section 5.1.15)

Note 1:– This test can be replaced by software revision control.

Note 2:– This test only applies to dispensers with electronic indicators.

- a) Lift the nozzle to activate the dispenser.
- b) Do not deliver the fuel – wait for the timeout.
- c) Check that the dispenser switches off and terminates the transaction within a period not greater than 120 seconds.
- d) Hang the nozzle for 5 seconds.
- e) Lift the nozzle to activate the dispenser and connect to the storage tank return line.
- f) Deliver a quantity of fuel.
- g) Stop the flow and note the time.
- h) Check that the dispenser switches off and terminates the transaction within a period not greater than 120 seconds.
- i) Hang the nozzle.
- j) ~~Record the result of the test of e) and h)~~Record the result of tests c) and h).

X.A-L-I.7.2.6 Air elimination check

- ~~a~~) ~~The~~ ~~l~~iquid pressurized line connected to the EUT shall enter the EUT via an electric controlled valve, activated by the operator's request for flow (dead man push button if needed).
- ~~a~~)~~b~~) During the idle state, the remaining liquid LPG is allowed to boil back to the storage tank via the storage tank return line for safety reasons. ~~The p~~urpose of this test is ~~t~~-o make sure that the volume of LPG under the gaseous phase will not alter the accuracy of ~~t~~-he measuring system at the next transaction.
- ~~b~~)~~c~~) Pre-condition the measuring standard – the volume of the check will be 20 literes minimal.
- ~~e~~)~~d~~) Leave the EUT idle for 3 minutes (the relaxing time for the air-separator to boil the liquid back to the storage tank).

- ~~e)~~ Lift the nozzle of the EUT while keeping the nozzle switch of the boot activated (to prevent pump activation), connect to the measuring standard~~l~~ for the high flow~~;~~.
- ~~d)f)~~ Activate the flow, simultaneously releasing the nozzle boot switch. ~~e~~Check that the display is reset to zero and stays at zero for 5 seconds, activate the flow immediately to achieve the maximum possible ~~flow-rate~~flowrate with no spillage, execute the accuracy check. The rResult shall be within the MPE for air-elimination.

X.A-L-I.7.2.7 Ancillary devices

X.A-L-I.7.2.7.1 Prepay

- eCheck of prepay function of dispenser.
 - ~~a)~~ The cCheck must be activated from the console controlling site.
 - ~~b)~~ Set the prepay volume to the target check volume (minimum 2 ~~x~~ MMQ) – to be done at the kiosk of the station.
 - ~~c)~~ Activate at the console, walk back to the dispenser and carry out the accuracy test, record the result.
 - ~~d)~~ Check the result versus the MPE requirements of ~~R-117~~R-117OIML R 117-1.
 - ~~e)~~ Record the pass/fail result. In the case of fail, record the reason if known.

X.A-L-I.7.2.7.2 -Printer for dispenser

- ~~i~~If the dispenser is equipped with its own printer, the check could take place during any previous check.
 - ~~a)~~ Check that the ticket issued reflects the information of the dial with no allowed difference.
 - ~~b)~~ ~~Record the pass/fail result on the initial verification paperwork~~Record the pass/fail result.

X.A-L-I.7.2.8 Temperature conversion (if applicable)

X.A-L-I.7.2.8.1 General

- ~~a)~~ During the check of the dispensers with temperature conversion, the special function/menu shall be available to read.
- ~~b)~~ Uncompensated volume.
- ~~c)~~ Temperature of the fuel from the EUT probe.
- ~~d)~~ Density if applicable.
- ~~e)~~ Correction tables or parameters, or signature of the used-tables used.
- ~~f)~~ The Pproper correction tables or parameters or signature of tables to be used shall be made available to the verification operator (e.g. corresponding to the fluid) so the calibration correction/check can be done properly.
- ~~g)~~ Proper training is needed for the verification operator to properly assess the results.

X.A-L-I.7.2.8.2 Test methods

X.A-L-I.7.2.8.2.1 General

Temperature conversion when applicable (measurement, probe position, see ~~clauses of OIML R-117~~clauses of OIML R 117-2, 6.3, ~~and OIML R-117~~and OIML R 117-1, 6.1.10 note 3).

FEDOR

X.A-L-I.7.2.8.2.2 Split EUT verification for first verification

These tests ~~is~~are done to check the accurate temperature reading of the fluid in the EUT.

- a) Install the reference probe (1) at the EUT temperature well.
- b) Disengage the temperature correction of the EUT.
- ~~(Note: _____ Refer to~~ the manufacturer's manual as this might be the way to have maintenance information displayed on the EUT dial such as the temperature of the fuel at the EUT conversion probe).
- c) Run the flow through the EUT at Q_{max} from the storage tank for at least 3 minutes to stabilize the fluid temperature and the EUT temperature (outgoing flow can be re-circulated back to the storage tank).
- d) Check the accurate temperature reading by comparing the temperature indicated by the EUT (converted signal from its own temperature probe) with ~~the reference~~ reference probe (1) inserted in the temperature well close to the instrument meter/transducer. ~~The m~~Maximum difference allowed is 1.3-3 °C.
- e) Stop the flow.
- f) Check the use of the correct conversion table (as per the type approval) in the conversion (calculator) arrangement.

X.A-L-I.7.2.9 Self-~~S~~ervice devices**X.A-L-I.7.2.9.1 Unattended mode – Differed ~~p~~Post payment**

- a) Initiate a transaction with the EUT (usually, done with a credit card system).
- b) Activate a few ~~liter~~litres of flow, and hang the nozzle.
- c) Check the good transmission of the corresponding transaction.
- d) Compare the display of the dispenser with the memorized (or printed when applicable) information at the SSD. This check can be also conducted ~~also~~ on the ticket printer at the credit card payment terminal when applicable.
- e) Check the good retrieving of the last transaction for the SSD memory when applicable.
- f) ~~Record the pass/fail result on the initial verification paperwork~~Record the pass/fail result. In the case of fail, record the reason.

X.A-L-I.7.2.9.2 Attended mode – Sale stacking – Immediate ~~P~~post payment

- a) Initiate a transaction with the EUT.
- 1)b) _____ Activate a few ~~liter~~litres of flow, and hang the nozzle.
- c) Initiate a new transaction with the EUT.
- 2)d) _____ Activate a few ~~liter~~litres of flow (different volume from the first transaction), and hang the nozzle.
- e) Try to initiate a new transaction with the EUT – it must be impossible (limited stacking to 2 transactions).
- 3)f) Check the good transmission of the corresponding transactions to the console/SSD.
- 4)g) _____ Check the good retrieving of both transactions from the SSD memory when applicable.

5)h) ~~Record the pass/fail result on the initial verification paperwork~~Record the pass/fail result. In the case of fail, record the reason.

FEDOR

Annex X.E

Test procedures for measuring systems (MS) for milk, beer and other foaming potable liquids (see ~~R 117~~OIML R 117-1, 5.6)

The technical aspects of the MS are explained [here](#). ~~This leads thus leading~~ to a better understanding in order to perform the tests correctly and to identify [any](#) problems, when an irregular performance of a MS occurs.


Technical aspects of milk MS

While [in their technical design](#) MS for the delivery of milk closely resemble, ~~in their technical design~~, conventional MS for the delivery of liquid petroleum and related products, in MS for the reception of milk the transfer point is defined by a constant level tank upstream of the meter. The air elimination device makes use of the constant level tank and is usually combined in one device. ~~T~~ the air elimination device may be separate if it is downstream of the constant level tank and before the meter. The level in the constant level tank before and after each measurement is established automatically.

Milk MS on road tankers and fixed milk MS (both for the reception) are usually designed in the same way, but the delivery line of a MS on a road tanker leads to a reception tank above the level of the meter (so that the meter will never run empty), whereas the delivery line of a stationary MS may lead to a reception tank beneath the level of the meter. ~~I~~ in this case, means in the delivery line are provided (e.g. a pressure maintaining valve, a special pipe geometry) which prevent the meter from running empty (see ~~OIML R 117-1~~, ~~clause~~ 5.6.2.6).


Main operational principles for the reception:

Suction of milk from a supply tank (milk churns, containers) into the air elimination device by a vacuum unit and transfer of milk from the air elimination device by a pump through the meter to the reception tank (see [Figure 1a](#)).



[Figure 1a:](#) ~~P~~Principal instrumentation of a milk measuring system, with suction by [a](#) vacuum

Suction of milk from a supply tank (milk churns, containers) by a pump and transfer of milk into the air elimination device and from the air elimination device through the meter to the reception tank (see [Figure 1b](#)).

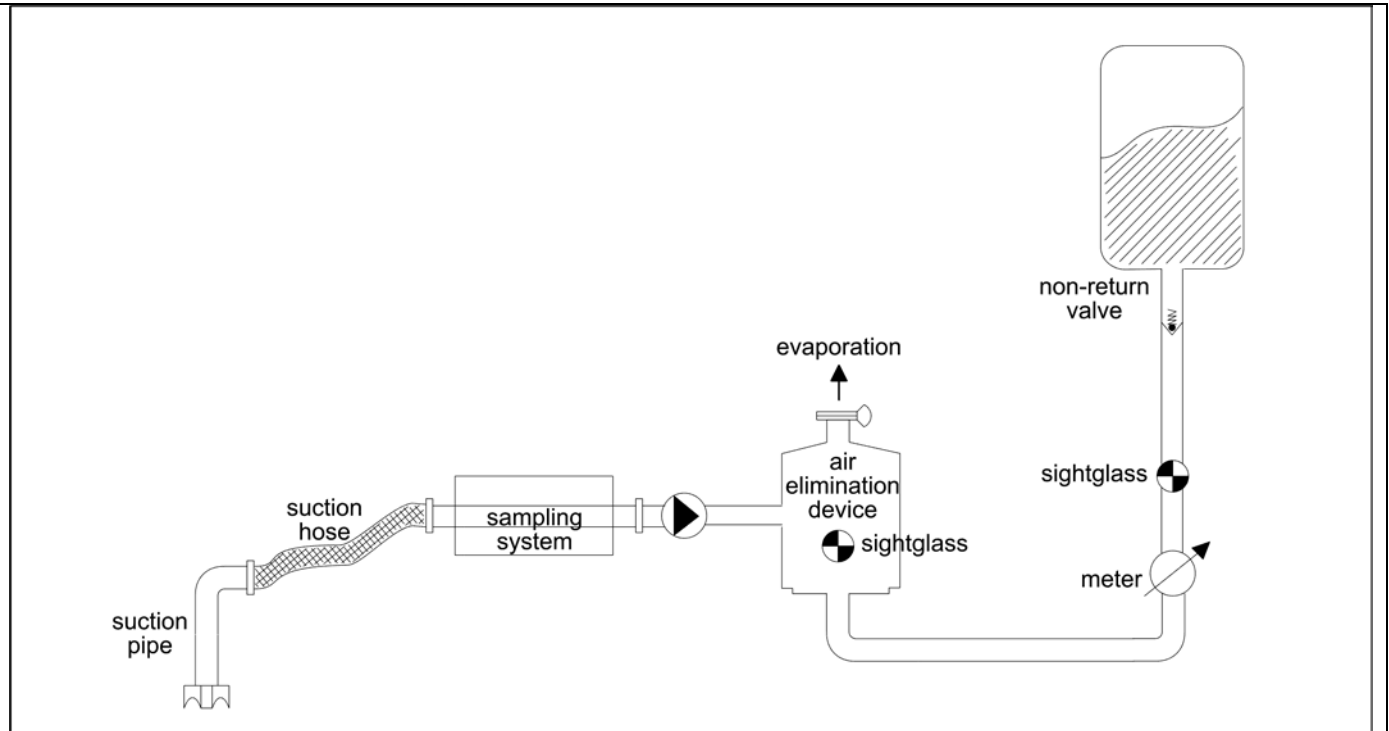[Figure 1b:](#) ~~P~~Principal instrumentation of a milk measuring system, with suction by [a](#) pump

Suction of [the](#) milk from a supply tank (milk churns, containers) into the air elimination device by a vacuum unit and transfer of [the](#) milk from the air elimination device by a pump through the meter to the reception tank. The air elimination device still acts as a transfer point, but air bubbles may pass it and enter the meter, but are registered by the sensors for the adequate correction of the liquid volume (see [Figure 1c](#)).

Note: Although this operational principle of a gas elimination device does not comply with a device described in [R117R-117/OIML R 117-1](#), 5.6.2 (constant level air elimination system upstream of the meter), [R117R-117/OIML R 117](#) is not intended to prevent the development of new technologies. Therefore, this operational principle is acceptable in the case where it yields equivalent results when tested under the same conditions as air elimination devices described in [R117R-117/OIML R 117-1](#), 5.6.2.

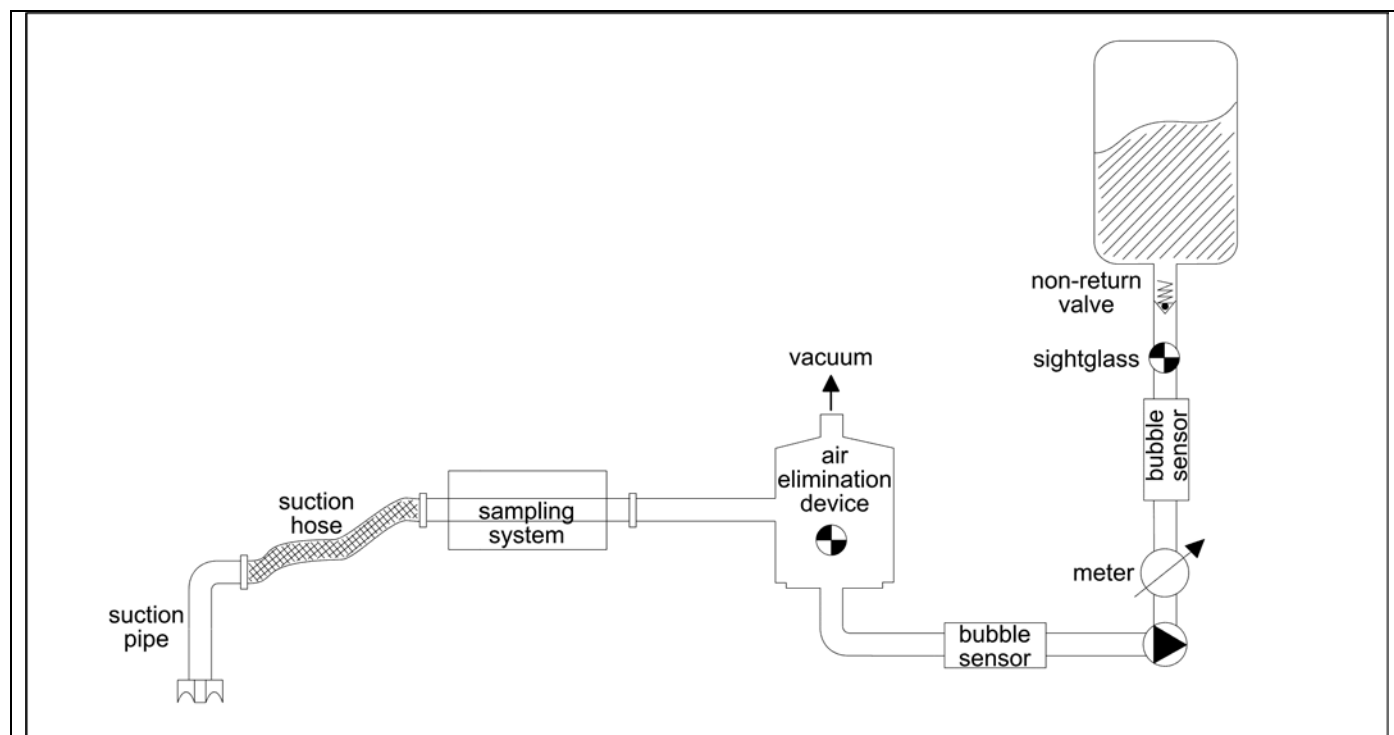


Figure 1c: – pPrincipal instrumentation of a milk measuring system, with bubble sensors

Specific instrumentation of a milk MS (given here in order of their installation)

Suction lines

The suction lines are automatically emptied at the finish of the reception. They are either designed as a rigid suction pipe connected to a flexible hose (to receive milk from milk churns) or as a flexible hose with a flange (for coupling the hose to a supply tank).

The hoses are reinforced and must allow the drainage at the finish of the reception.

A MS may have more than only one suction line (in such a case the suction lines are interlocked against simultaneous usage).

A suction line may have one or several diversion lines (e.g. for pumping the milk by the aid of the pump of the MS into a trailer); such diversion lines are locked during the reception (the interlock shall be verified).

A suction line may have a connection with a manual valve (for emptying and rinsing).

Possible problems:

(Small) cracks in the hoses and defect gaskets at the couplings/joints of the hoses generate air bubbles which cannot be removed by the air elimination device; an unusual quantity of foam is present in the air elimination device at the end of a transaction (visible through the sight glass of the air elimination device).

Sampling systems (usually arranged in the suction line)

For quality investigations (e.g. fat content, contamination) the MS usually has ~~ave~~ devices in the suction line which automatically divert a small volume sample from the received quantity.

Examples of the design of sampling systems:

- A pre-determined volume is diverted into a container where the milk is stirred, and – after diverting a small volume of the stirred milk into a flask ~~–~~ returned to the MS upstream of the meter (the return

may also be accomplished after the set of the level in the air elimination device, so that the pump will be re-started for a short period to take over the diverted quantity.

- The product sample is diverted by a pump (which is controlled by the meter of the MS or by an additional meter/sensor mounted in the suction line) and directly injected into a sample vial.

Temperature sensor(s)

Only for documentation, not under metrological control.

Possibly installed in the suction line.

Pumps

Pumps on road tankers are driven either by the auxiliary drive of the vehicle's gearbox or by an electric motor connected to an exterior power supply.

Figures 1a and 1c show how the milk is sucked into the air elimination device by a vacuum (generated e.g. by one or more ejectors, by a vacuum pump). A pump located downstream of the air elimination device (usually a rotary pump, not self-priming) transfers the milk through the meter into the reception tank, until the reception comes to its finish and the level at the air elimination device is set to the transfer point. The pump is controlled automatically by the filling level in the air elimination device.

Figure 1b shows how the milk is pumped into the air elimination device by a pump located upstream of the air elimination device (usually impeller centrifugal pump = vane type pump, self-priming). The pump transfers the milk through the air elimination device and the meter into the reception tank, until the reception comes to its finish and the level at the air elimination device is set to the transfer point. The pump is controlled automatically by the filling level in the air elimination device.

Possible problems:

- A leaky shaft-seal of the pump generates small air bubbles which cannot be removed by the air elimination device; an unusual quantity of foam is present in the air elimination device at the end of a transaction (visible through the sight glass of the air elimination device).
- Increasing the speed of the pump (which on road tankers is driven by the auxiliary drive of the vehicle's gear) may lead to a flowrate outside of the approved flowrate range.

Increasing the speed of the pump may cause a mixture of air and milk which is outside the approved capability of the air elimination device.

Gears for driving the pump (by their auxiliary drive) may be constructed in this way that they can split the gears, so that 2 different speeds of the auxiliary drive are settable. Therefore, care shall be taken to set the gear such that during the tests the maximum possible flowrate is achieved.

Control units for the transaction procedure

The control of sensors, activators and pumps as well as the selection and control of the path of the liquid is usually performed by a store-programmed control (SPC) which may either be designed as a separate unit or may be incorporated into the software/hardware part of the ECID.

For the correct interaction of all parts of the instrumentation leading to a correct performance of the MS, the SPC has a complex system of settable parameters (e.g. parameters for pressure control of the vacuum, pump speed depending on the filling level at the air elimination device, time variables for pump follow-up).

Temporary Note: Although some of these parameters may be sensitive to the performance of the MS and must not be changed after the test, it is common practice not to secure them in the SPC against unauthorized modification.

At any rate it must be possible to secure device specific parameters (such as the calibration factor of the meter, the ID of the measuring system and its components, the settings of a dip stick in the air elimination

device, the volume required to fill the measuring system - colloquially called “flood volume” or “dry start priming volume”) against unauthorized modification.

It may happen that during the tests a reduction of the flowrate (e.g. by the control unit, by the ratio of the gear) yields better measuring results, but the MS in service is operated at higher flowrates; therefore care shall be taken that the tests are performed at the maximum attainable flowrate of the MS.

Air elimination device

For the elimination of air, ~~R-117~~OIML R 117-1 requires the following devices:

A **gas separator** shall be provided when the pressure at the pump inlet may, even momentarily, fall below the atmospheric pressure (the liquid does not supply the pump by gravity).

Examples:

- MS with pumped flow, with an underground supply tank;
- MS with pumped flow, with an overground supply tank, but with supply lines above the level of the supply tank;
- MS with pumped flow, with a low suction head;

when the pump is of the self priming type. Centrifugal pumps and vane type pumps are usually of the non-self priming type, but may also be designed as a self priming type.

As an alternative solution for a gas separator the manufacturer may present e.g.

- a pressure sensor monitoring that the pressure is always above the atmospheric pressure,
- an air detector with a venting device.

A **gas extractor** shall be provided when the pressure at the pump inlet is always greater than the atmospheric pressure, and if air pockets liable to have a specific effect greater than 1 % of the MMQ can occur (if such air pockets can also occur at flow conditions under which a gas separator is mandatory, this gas separator shall also be approved as a gas extractor). Air pockets are likely to be introduced into the pipework when the supply tank becomes empty.

A **special gas extractor**, mainly used for delivery MS on road tankers, is principally intended to prevent measurement errors which may arise from the complete emptying of one compartment. It must also separate and continuously remove introduced air, although to a lesser degree than a gas separator. Installing a special gas extractor is subject to supply conditions.

~~R-117~~OIML R 117-1, 2.10.2 and 2.10.3 also consider supply conditions under which an air elimination device is not needed at all, especially when the meter is supplied by gravity without the use of a pump. But even then, the pressure at the meter inlet may fall below the atmospheric pressure, e.g. when the inlet line of the meter bears constrictions < nominal diameter of the meter inlet.

~~Please n~~Note that ~~R-117~~OIML R 117-1, 2.10 does not state any further requirements on the performance of air elimination devices except that the air must be evacuated automatically unless a device is provided which automatically either stops or sufficiently reduces the flow of liquid when there is a risk of air entering the meter (~~R-117~~OIML R 117-1, 2.10.7.1). This requirement is met by types of air elimination devices, which close a valve downstream of the meter during the evacuation of air.

Air elimination devices are usually designed as a tank serving as an air elimination device with a built-in constant level tank (which serves as the transfer point) and located upstream of the meter. The level is established automatically.

Usually, the constant level at the transfer point before and after the measurement can be monitored by a sight glass with two marks (the level is considered to be constant when it settles within the two marks); some types

of air elimination devices have a built-in automatic level gauge (e.g. designed as a dip stick) which measures the level before and after the transaction and provides an adequate volume correction so that it is not necessary to visually check the constant level before and after each reception.

The volume required to fill the MS (colloquially called “flood volume” or “dry start priming volume”) is either stored as a parameter in the ECID or marked on the name plate of the MS.

De-gassing lines of the air elimination device usually do not have any closure devices being operated manually.

Instead of the air elimination device described above, the MS may have a device serving as a transfer point together with bubble sensors (see [Figure 1c](#)).


The transfer point device controls the intake process at the start and finish of the transaction; when air bubbles pass the transfer point device they are registered by the bubble sensor (located at the inlet side of the pump), which adjusts the pump speed accordingly, and are quantified by the second bubble sensor (located at the outlet side of the meter) with an adequate correction of the milk volume.

The SW of the calculation program of the bubble sensor is subject to metrological control and shall be validated and secured.

Note: Although this principle of a gas elimination device does not comply with the devices mentioned in [R-117OIML R 117-1](#), 2.10 and 5.6, [R-117OIML R 117](#) does not intend to prevent new technologies (see [R-117OIML R 117-1](#), 1.1 and B.2.10.2).

In order to minimize mixing when receiving different grades of milk, an MS may have two air elimination devices (see [Figure 2](#)), supplied by either a common suction line or by 2 suction lines, and connected to one meter.

In MS with two air elimination devices, different flood volumes may occur.

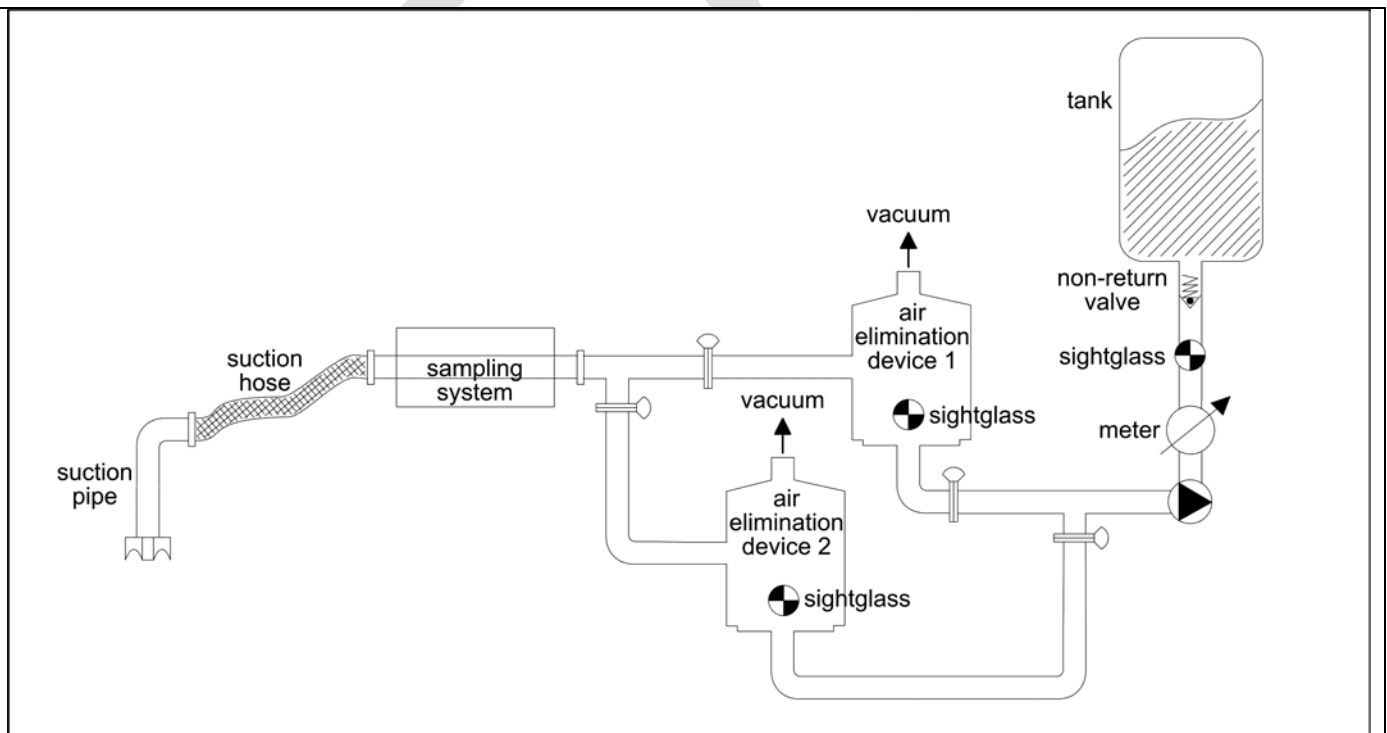

[Figure 2](#): Principal instrumentation of a milk MS with two air elimination devices

Possible problems:

- Because air elimination devices are sensitive to the ~~used~~-product used (cream and foam in the air elimination device may hamper its correct function, especially when it contains mechanical parts such as a floater), only accuracy tests with the intended liquid will yield representative results, but not accuracy tests with water.
- The suction of milk having been stored without stirring and pumping generates solid substances and consequently a malfunction of the air elimination device (measurement errors, repeatability problems). Milk ~~beneath~~-below 5 °C or skimmed milk generates foam and consequently a malfunction of the air elimination device.

Meters

For ~~the~~ ease of cleaning of the MS (cleaning in process - CIP) usually electromagnetic meters are installed.

Electromagnetic meters can be tested on a test bench with water; ~~the~~ the usage of milk will then shift the error curve approximately by + 0.15 % (this difference is not due to viscosity and density, but probably due to a microfilm of fat on the meter walls including electrodes, which changes ~~somewhat~~ the conductivity somewhat).

Equipment for the complete filling

- A non-return valve between the air elimination device/constant level tank and the meter, to prevent backflow from the meter (e.g. in cases when the meter is located above the transfer point).
- A non-return valve between the meter and the receiving tank (in order to prevent reverse flow over the meter), optionally combined with a pressure maintaining valve (in order to care for a proper setting of the liquid level in the constant level tank).

Possible problems:

- A leakage of the non-return valve (e.g. due to the suction of gasket parts from the upstream pipes) leads to ~~non~~-repeatability measurement results and/or changes of the liquid level in the sight glass (remedyied by dismounting the non-return valve and cleaning it).
- Sight glass at the outlet side of the meter.

Branches

Optionally, MS on road tankers have a branch to transport milk from their reception tank to a trailer (see Figure 3):

The milk is sucked from the delivery line via an own pipe to the suction side of the pump and delivered via a connection downstream of the pump. Valves with an automatic interlock safeguard that this transfer has no influence on the normal operation of the MS.

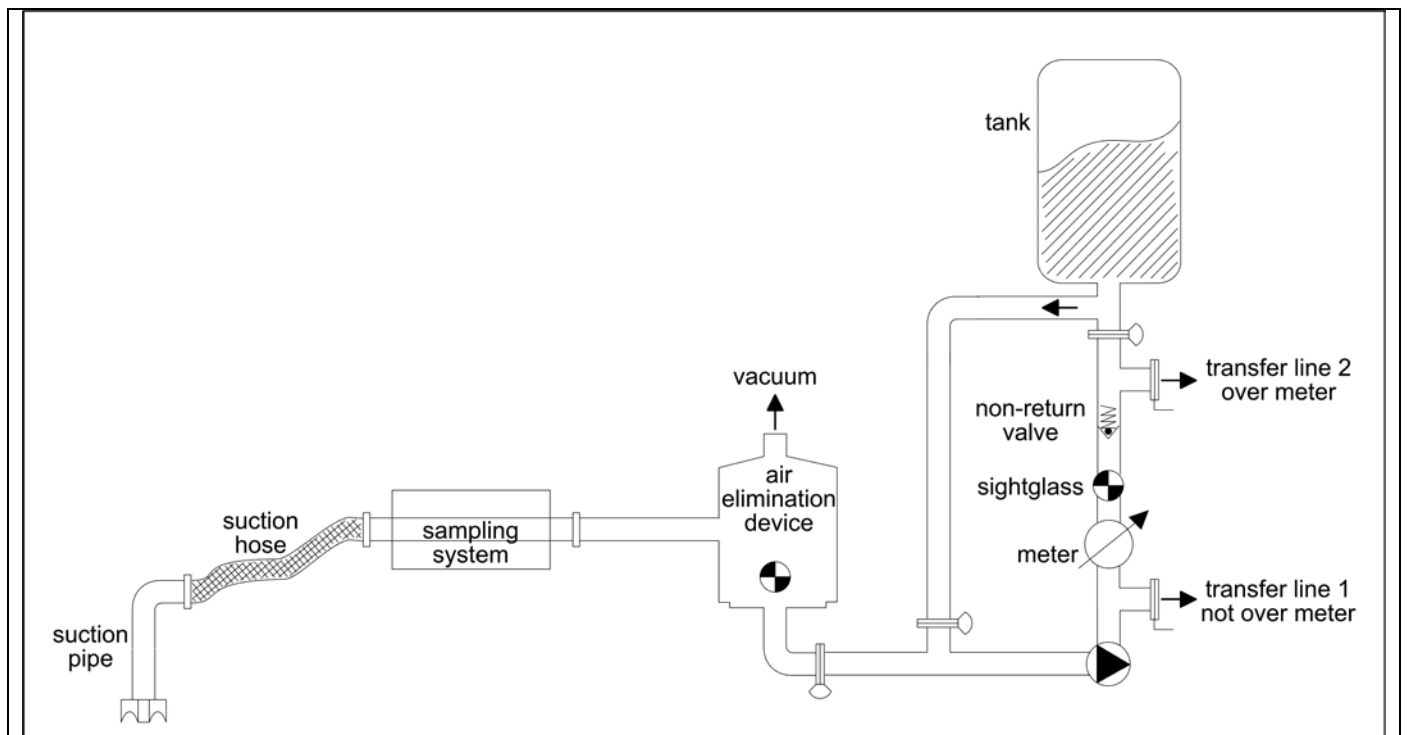


Figure 3: Principal instrumentation of a milk MS, with transfer line from tank to trailer

Technical aspects of MS for beer and other foaming potable liquids

MS on road tankers and stationary MS are usually designed in a similar way.

They are mainly designed for ~~the~~ delivery, but may also be foreseen for ~~the~~ reception under metrological control.


The MS are full hose systems. The nozzle at the end of the hose is the transfer point.

For the purpose of conservation, beer and other foaming potable liquids contain carbonic acid. Free surfaces in the MS (e.g. in the supply tank and in the reception tank) need a gas pressure atmosphere (pressure ≥ 0.5 bar) to prevent the release of gas dissolved in the liquid (commonly CO₂, which also prevents the oxidation of the liquid).

Usually, the MS has a pump which is supplied by the gas pressure in the supply tank, but the MS may also be designed as a pressurized system.

The MS foresees a constant pressure during the whole delivery.

Specific instrumentation of a MS (given here in order of their installation):

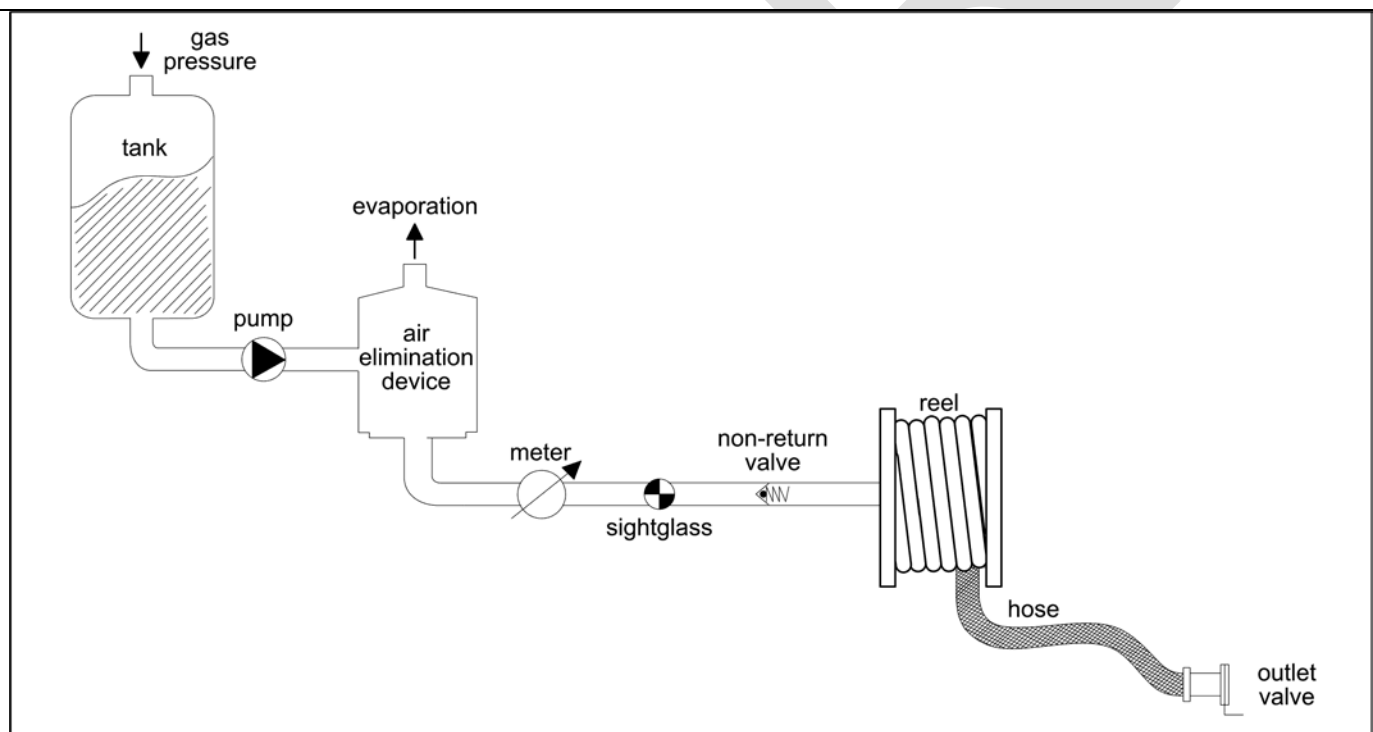

~~Fig-ure~~ 4: ~~p~~Principal instrumentation of measuring system for beer, for delivery only

Supply tank (normally pressurized by a CO₂-atmosphere, common pressure ≥ 0.5 bar), consisting of one or ~~of~~ several chambers, followed by suction lines with a pump (~~pump~~ additionally to the supply of the meter by the gas pressure in the supply tank, in order to overcome the back pressure due to lines and hoses and to vertical height).

Optional equipment

Temperature sensor, manometer, which may be installed at any site of the MS and which is not under metrological ~~control~~.

Control unit for the transaction procedure

The control of sensors, activators and pumps as well as the selection and control of the path of the liquid is usually performed by a store-programmed control (SPC) which may either be designed as a separate unit or may be incorporated into the software/hardware part of the ECID.

For the correct interaction of all parts of the instrumentation leading to a correct performance of the MS, the SPC has a complex system of settable parameters (e.g. parameters for pressure control).

At any rate it must be possible to secure device specific parameters (such as the calibration factor of the meter, and the ID of the measuring system and its components) against unauthorized modification.

Gas elimination device

Due to the design of such MS (supply tank with pressurized atmosphere at a pressure ≥ 0.5 bar) the pressure at the pump inlet is always > 1 bar and therefore no pressure drop at the pump inlet below atmospheric pressure can occur. Furthermore, de-gassing is not possible, and therefore air or gas slightly mixed with the liquid will not occur. Even if de-gassed portions of carbonic acid might occur (e.g. due to a Venturi effect), they will recombine immediately with the liquid.

So the gas elimination device must only be capable of removing gas pockets when the supply tank gets becomes empty (the gas elimination device works as a gas extractor). ~~I~~ Instead of a gas elimination device, the MS may be equipped with an appropriate device which prevents the entry of gas from the supply tank (e.g. level sensor at the outlet of the supply tank, which actuates the closure of a delivery valve).

Usually, manually operated closure devices are not present in the de-gassing line of the gas elimination device. They may be acceptable in the case ~~that~~ when the gas elimination device registers gas, the delivery is automatically stopped until the gas is removed over the manually operated closure device.

Equipment for ~~the~~ complete filling

- Sight glass at the outlet side of the meter;
- ~~n~~Non return valve(s) to avoid backflow over the meter;
- ~~p~~Pressure maintaining valve(s) to avoid de-gassing of the liquid.

Hoses, with outlet valve

Branches

Optionally, MS on road tankers may have a branch to pump back the liquid from a customer's tank (see Figure -5).

The liquid is sucked in from the hose via an own pipe to the suction side of the pump and delivered via an own pipe downstream of the pump to the supply tank of the road tanker. Valves and an automatic interlock safeguard that this reception procedure has no influence on the normal operation of the MS.

Measures are provided to safeguard that all parts of the MS (including the hose) remain full after the reception.

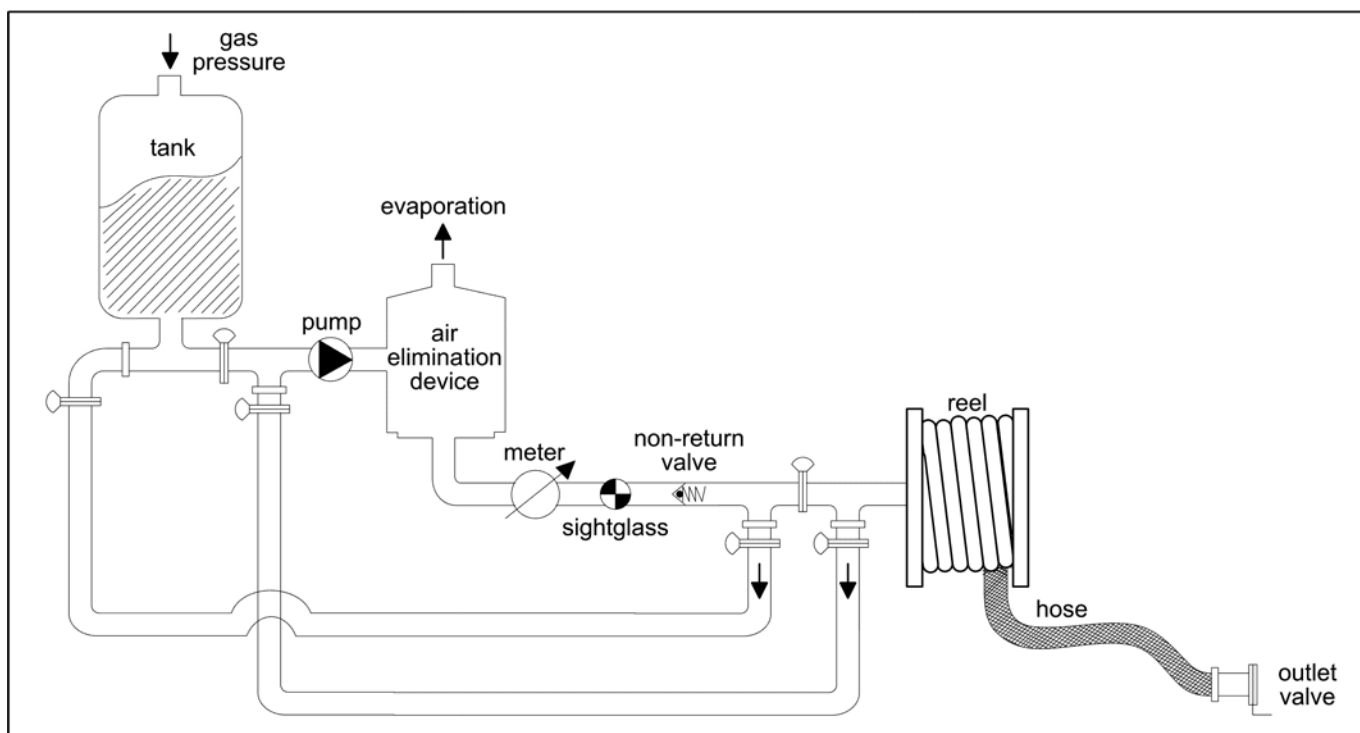


Figure 5: Principal instrumentation of measuring system for beer, also for reception

Annex X.G - Fuelling of aircraft

X.G.1 Technical aspects of fuelling of aircraft

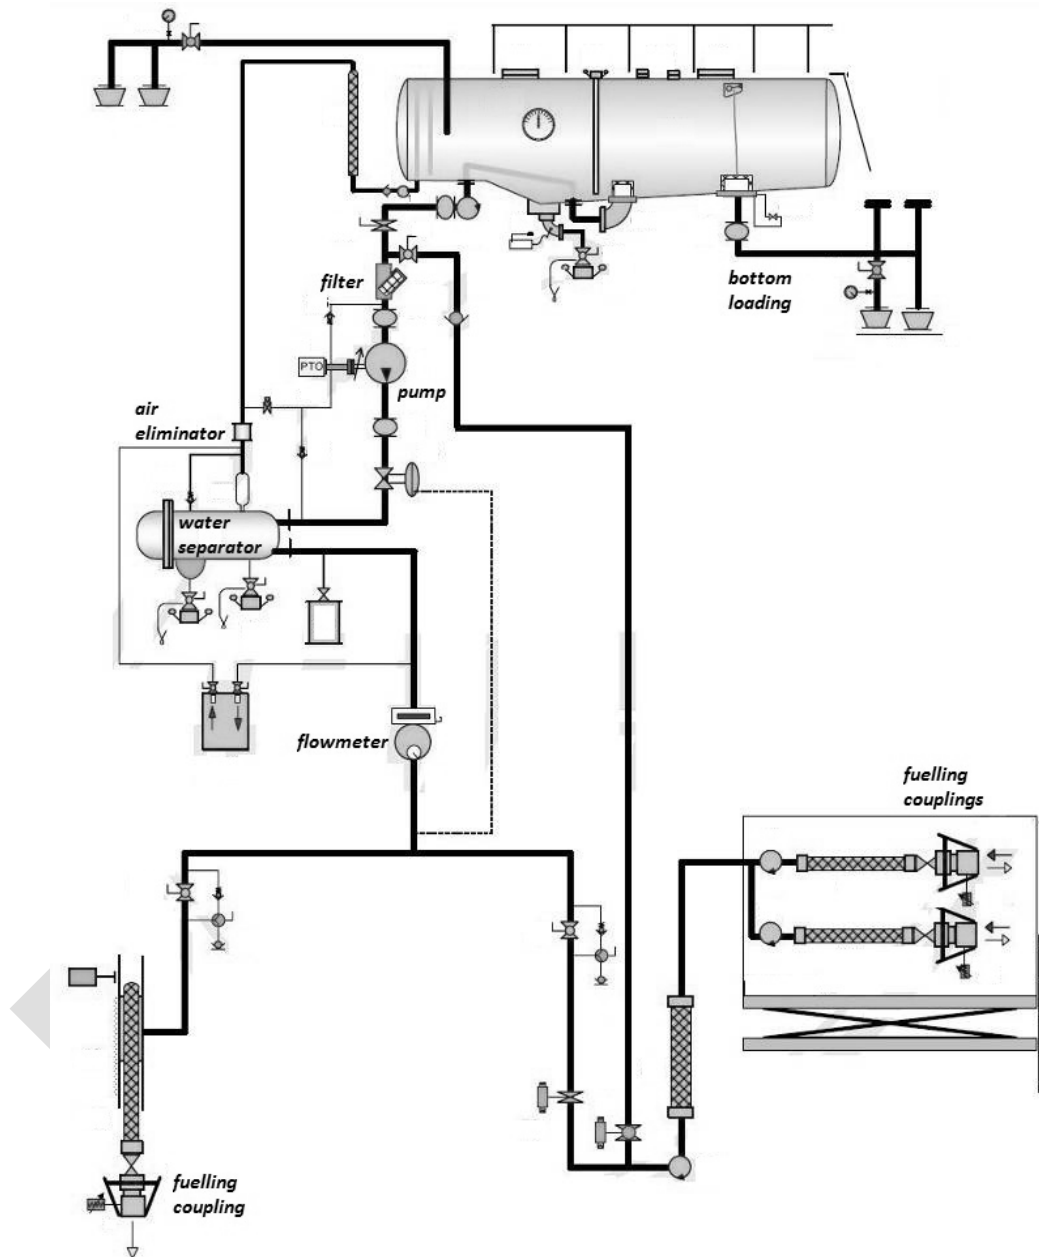


Figure X.G.1 Schematic of typical aircraft fuelling system

X.G.3 Metrological controls and performance tests for initial verification

Before conducting verification tests it is necessary to complete a full design evaluation of the measuring system intended for the fuelling of aircraft.

For initial verification, the same test procedures shall be used as the system tests for type approval, except the items gas elimination devices test and variation in the internal volume of the hose test.

~~For initial verification, the same test procedures shall be used as the system tests for type approval, except the items G.4 and G.5.3.~~

For safety reasons, special grounding devices may be needed to ensure the safety and security of the fuelling operations.

The requirements of ~~sections~~ 5.8.1.2, 5.8.2.3, 5.8.3.1.3, 5.8.3.2, 5.8.3.3.1 and 5.8.3.3.2 of ~~R-117~~R-117OIML R 117-1 (as applicable) shall be fulfilled.

X.G.3.1 Accuracy test of the complete measuring system

These tests include:

- Accuracy tests at maximum achievable flowrate-;
- Accuracy tests at 0.5—0.7 of the maximum achievable flowrate -(optionally for electronic meters)-;
- Accuracy tests at Q_{min} -; and-;
- Tests on the minimum measured quantity (with maximum specified hose length).;

~~Testing is completed in accordance with Section 5. These tests include:~~

~~Accuracy tests at Q_{min} and -;Tests on the minimum measured quantity (with maximum specified hose length);~~**X.G.4.4 Additional test procedures for the complete measuring system intended for the refuelling of aircraft**

X.G.4.1.1 Common tests for all measuring systems intended for refuelling of aircraft

X.G.4.1.1.1 Object of the test

To determine the accuracy of the quantity indication of the stationary or mobile measuring system intended for refuelling of aircraft during delivery.

X.G.4.1.2 ~~X.G.4.1.3~~ Test procedure

~~Testing is completed in accordance with paragraph G.2.5.1.2 Test procedure (Type approval)- of Annex G with the exception of the MMQ test, if the MMQ is smaller than 500 L.~~

~~The delivery starts from an appropriate source of delivered liquid (pipeline or tank upstream of the measuring system)-.~~

~~It is necessary to ensure that liquid level in tank remains above its lowest permissible level during testing-~~

FEDOR